

E L E K T A

# Elekta Limited

## DICOM Conformance Statement

For

Elekta XVI

Release 3.5

Document Number: 4513 350 0900  
Version: 2.0  
Date: 15/06/2005

© 2005 Elekta Limited.  
All rights reserved.

**Issued By:**

Elekta Limited  
Linac House  
Fleming Way  
CRAWLEY  
West Sussex RH10 9RR  
United Kingdom

Tel: +44 (0)1293 544422

Fax: +44 (0)1293 654321

<http://www.elekta.com>

# LIST OF CONTENT

<b>1</b>	<b><u>INTRODUCTION</u></b>	<b>5</b>
1.1	<u>SCOPE AND FIELD OF APPLICATION</u>	5
1.2	<u>INTENDED AUDIENCE</u>	5
1.3	<u>CONTENTS AND STRUCTURE</u>	5
1.4	<u>USED DEFINITIONS, TERMS AND ABBREVIATIONS</u>	5
1.5	<u>REFERENCES</u>	5
1.6	<u>IMPORTANT NOTES TO THE READER</u>	6
<b>2</b>	<b><u>IMPLEMENTATION MODEL</u></b>	<b>7</b>
2.1	<u>APPLICATION DATA FLOW DIAGRAM</u>	7
2.2	<u>FUNCTIONAL DEFINITION OF APPLICATION ENTITY</u>	7
2.3	<u>SEQUENCING OF REAL-WORLD ACTIVITIES</u>	7
2.4	<u>ELEKTA SYNERGY™ AE SPECIFICATION</u>	9
2.4.1	<u>The Dicom Import Validation Tool mechanism:</u>	9
2.4.2	<u>Association Establishment Policies</u>	9
2.4.3	<u>Association Initiation Policy</u>	10
2.4.4	<u>Association Acceptance Policy</u>	14
<b>3</b>	<b><u>COMMUNICATION PROFILES</u></b>	<b>17</b>
3.1	<u>SUPPORTED COMMUNICATION STACKS</u>	17
3.2	<u>TCP/IP STACK</u>	17
3.3	<u>PHYSICAL MEDIA SUPPORT</u>	17
<b>4</b>	<b><u>EXTENSIONS/SPECIALISATIONS/PRIVATISATIONS</u></b>	<b>18</b>
<b>5</b>	<b><u>CONFIGURATION</u></b>	<b>19</b>
5.1	<u>AE TITLE/PRESENTATION ADDRESS MAPPING</u>	19
5.1.1	<u>Local AE Titles and Presentation Addresses</u>	19
5.1.2	<u>Remote AE Titles and Presentation Addresses</u>	19
5.2	<u>CONFIGURABLE PARAMETERS</u>	19
5.2.1	<u>Communication Parameters</u>	19
<b>6</b>	<b><u>SUPPORT OF EXTENDED CHARACTER SETS</u></b>	<b>20</b>
<b>A.</b>	<b><u>APPLIED RT PLAN IOD AND MAPPING TO ELEKTA SYNERGY™ DATABASE</u></b>	<b>21</b>
A.1	<u>RT PLAN IOD MODULES</u>	21
<b>B.</b>	<b><u>APPLIED RT STRUCTURE SET IOD AND MAPPING TO ELEKTA SYNERGY™ DATABASE</u></b>	<b>32</b>
B.1	<u>IMPORT OF RT STRUCTURE SET</u>	32
B.2	<u>RT STRUCTURE SET IOD MODULES</u>	32
<b>C.</b>	<b><u>APPLIED CT IMAGE IOD AND MAPPING TO ELEKTA SYNERGY™ DATABASE</u></b>	<b>37</b>
C.1	<u>IMPORT OF CT IMAGE</u>	37
C.2	<u>EXPORT OF CT IMAGE</u>	41
<b>D.</b>	<b><u>APPLIED RT IMAGE IOD AND MAPPING TO ELEKTA SYNERGY™ DATABASE</u></b>	<b>46</b>
D.1	<u>IMPORT OF RT IMAGE</u>	46
D.2	<u>RT IMAGE IOD MODULES</u>	46
<b>E.</b>	<b><u>APPLIED SC IMAGE IOD AND MAPPING TO ELEKTA SYNERGY™ DATABASE</u></b>	<b>53</b>
E.1	<u>IMPORT OF SC IMAGE</u>	53
E.2	<u>EXPORT OF SC IMAGE</u>	57

**F.** **EXTENDED IMAGE IMPORT CAPABILITY** .....61

**F.1** **C-STORE CONFORMANCE WHEN EXTENDED IMPORT IS ENABLED**.....61

**G.** **C-STORE RESPONSE STATUS CODES**.....62

# 1 Introduction

This chapter provides general information about the purpose, scope and contents of this Conformance Statement.

## 1.1 Scope and field of application

The scope of this DICOM Conformance Statement is to facilitate data exchange with equipment of Elekta Limited. This document specifies the compliance to the DICOM standard (formally called the NEMA PS 3.X-2003 standards). It contains a short description of the applications involved and provides technical information about the data exchange capabilities of the equipment. The main elements describing these capabilities are the supported DICOM Service Object Pair (SOP) Classes, Roles, Information Object Definitions (IOD) and Transfer Syntax's.

The field of application is the integration of the Elekta Limited equipment into an environment of medical devices.

This Conformance Statement should be read in conjunction with the DICOM standard and its addenda.

## 1.2 Intended audience

This Conformance Statement is intended for:

- (potential) customers,
- system integrators of medical equipment,
- marketing staff interested in system functionality,
- software designers implementing DICOM interfaces

It is assumed that the reader is familiar with the DICOM standard.

## 1.3 Contents and structure

The DICOM Conformance Statement is contained in chapter 2 through 6 and follows the contents and structuring requirements of DICOM PS 3.2-2003. Additionally, the Appendices following chapter 6 specify the details of the applied IODs, SCP-specific status codes and extended configuration details.

## 1.4 Used definitions, terms and abbreviations

- DICOM definitions, terms and abbreviations are used throughout this Conformance Statement. For a description of these, see DICOM PS 3 2003.
- The word Elekta in this document refers to Elekta Limited.
- The phrase Elekta Synergy™ in this document refers to the XVI application release 3.5.

## 1.5 References

[DICOM PS 3 2003]

The Digital Imaging and Communications in Medicine (DICOM) standard:  
NEMA PS 3.X (X refers to the part 1 - 13) and Supplements.  
National Electrical Manufacturers Association (NEMA) Publication Sales  
1300 N. 17th Street, Suite 1847  
Rosslyn, Va. 22209, United States of America

## 1.6 Important notes to the reader

This Conformance Statement by itself does not guarantee successful interoperability of Elekta equipment with non-Elekta equipment. The user (or user's agent) should be aware of the following issues:

- **Scope**

The goal of DICOM is to facilitate inter-connectivity rather than interoperability. Interoperability refers to the ability of application functions, distributed over two or more systems, to work successfully together. The integration of medical devices into a networked environment may require application functions that are not specified within the scope of DICOM. Consequently, using only the information provided by this Conformance Statement does not guarantee interoperability of Elekta equipment with non-Elekta equipment. It is the user's responsibility to analyse thoroughly the application requirements and to specify a solution that integrates Elekta equipment with non-Elekta equipment.

- **Validation**

Elekta equipment has been carefully tested to assure that the actual implementation of the DICOM interface corresponds with this Conformance Statement. Where Elekta equipment is to be linked to non-Elekta equipment, the first step is to compare the relevant Conformance Statements. If the Conformance Statements indicate that successful information exchange should be possible, additional validation tests will be necessary to ensure the functionality, performance, accuracy and stability of prescription and prescription related data. Prospective users may contact Elekta for up-to-date information regarding available validation status and any known compatibility issues with specific 3<sup>rd</sup> party vendors. Ultimately, however, it is the responsibility of the user (or user's agent) to specify an appropriate test suite and to carry out additional validation tests on combinations of equipment used within the users environment. In particular integrators should not assume that the Elekta equipment would always be able to detect all forms of invalid data originating from 3<sup>rd</sup> party equipment.

- **New versions of the DICOM Standard**

The DICOM Standard will evolve in future to meet the user's growing requirements and to incorporate new features and technologies. Elekta is actively involved in this evolution and plans to adapt its equipment to future versions of the DICOM Standard. In order to do so, Elekta reserves the right to make changes to its products or to discontinue its delivery. The user should ensure that any non-Elekta provider linking to Elekta equipment also adapts to future versions of the DICOM Standard. If not, the incorporation of DICOM enhancements into Elekta equipment may lead to loss of connectivity and/or incompatibility.

## 2 Implementation Model

The Elekta Synergy™ SCP stores received DICOM message information in the Transit Dicom Database. The location of the Transit Dicom database is specified in the local Elekta Synergy™ configuration file  
Elekta Synergy™ is a networked information system comprising Control Systems and Operators Consoles for use with Elekta Linear Accelerators, together with a centralised Patient database for Image guidance therapy and Portal imaging purposes.

### 2.1 Application Data Flow Diagram

Elekta Synergy™ behaves as a single Application Entity (AE). The related Implementation Model is shown in Figure 1.


### 2.2 Functional definition of Application Entity

Elekta Synergy™ application entity acts as Service Class Provider (SCP) Storage Service Class, Service Class User (SCU) Storage Service Class and SCU Query/Retrieve Service Class.

The Application Entity is active when the Elekta Synergy™ system is switched on.

### 2.3 Sequencing of Real-World Activities

Not applicable.

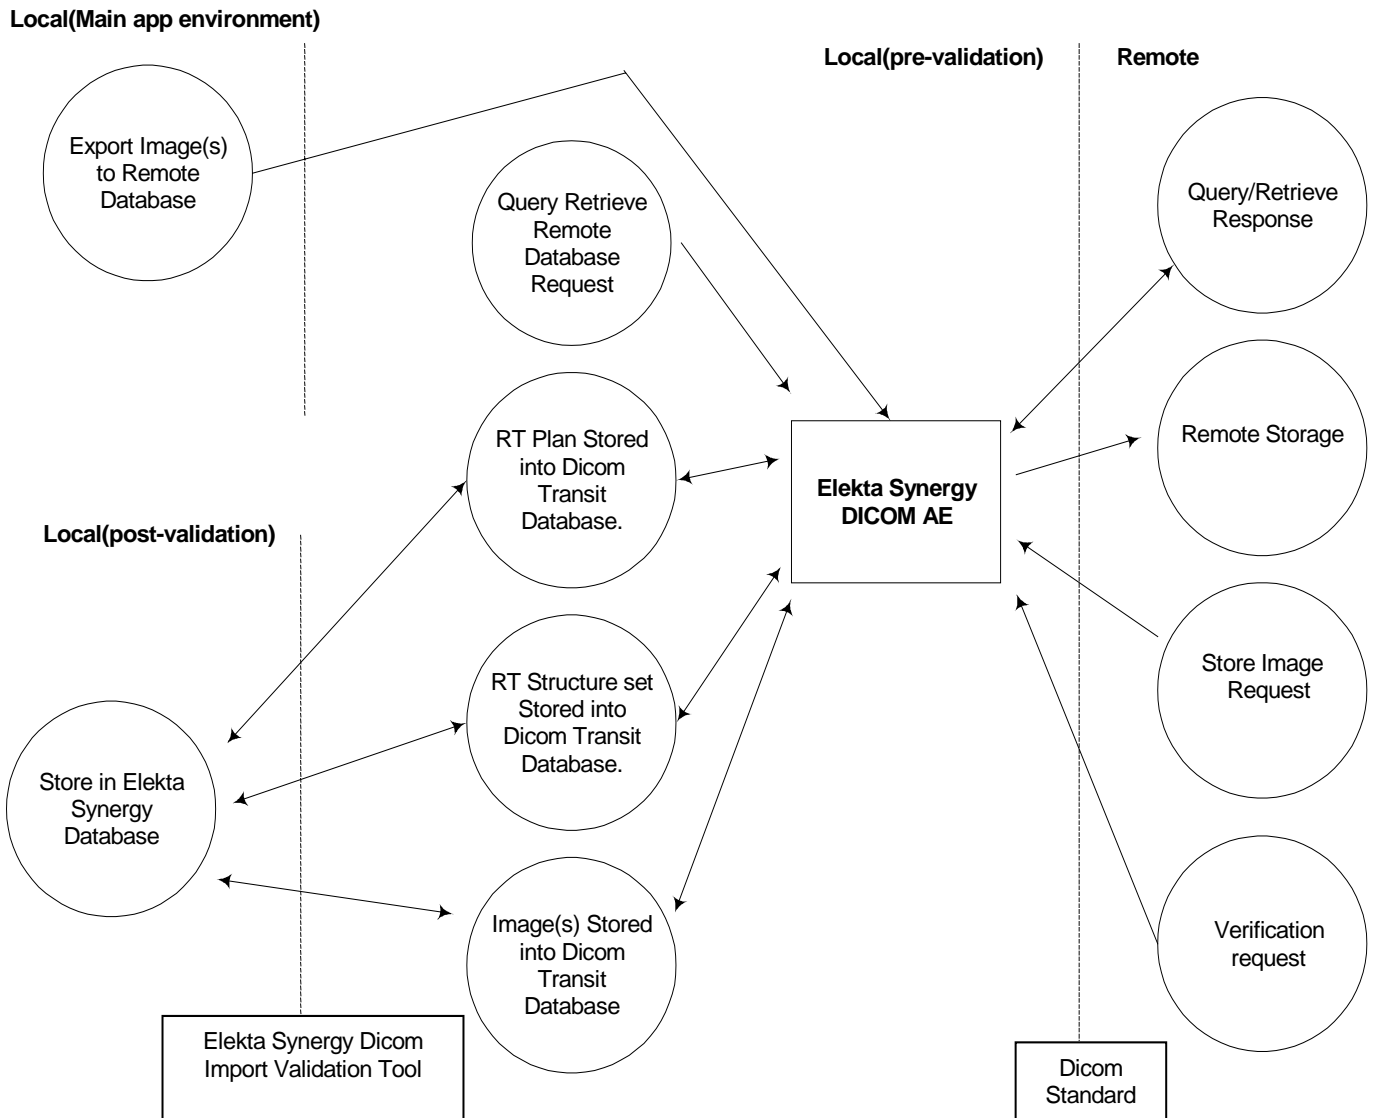

**Figure 1 Elekta Synergy™ Dicom import implementation model**



AE Specifications

## 2.4 Elekta Synergy™ AE Specification

Elekta Synergy™ Application Entity provides Standard Conformance to the following DICOM V3.0 SOP classes as an SCP:

**Table 1 SOP Classes supported by Elekta Synergy™ as SCP**

SOP Class Name	UID
RT Plan Storage - STORE	1.2.840.10008.5.1.4.1.1.481.5
RT Structure Set Storage - STORE	1.2.840.10008.5.1.4.1.1.481.3
RT Image Storage - STORE	1.2.840.10008.5.1.4.1.1.481.1
SC Image Storage - STORE	1.2.840.10008.5.1.4.1.1.7
CT Image Storage - STORE	1.2.840.10008.5.1.4.1.1.2
Verification	1.2.840.10008.1.1

Elekta Synergy™ Application Entity provides Standard Conformance to the following DICOM V3.0 SOP classes as an SCU:

**Table 2 SOP Classes supported by Elekta Synergy™ as SCU**

SOP Class Name	UID
Patient Root Query/Retrieve Info Model - FIND	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Query/Retrieve Info Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2
SC Image Storage - STORE	1.2.840.10008.5.1.4.1.1.7
CT Image Storage - STORE	1.2.840.10008.5.1.4.1.1.2

### 2.4.1 The Dicom Import Validation Tool mechanism:

All Dicom data received will be first saved as Dicom files into a local Elekta Synergy™ DICOM Transit database. The location of this database is settable through Elekta Synergy™ sri.ini initialisation file. The success of the transfer into the Elekta Synergy™ DICOM Transit database will depend on the results of a Dicom validation test (test the Dicom object is valid as far as Dicom is concerned) and the compliance to our internal Validation rules (described in Appendix A).

To move the Dicom messages from the Elekta Synergy™ DICOM Transit database to the Main Elekta Synergy™ database the user will use the Elekta Synergy™ Dicom Import Validation Tool (DIVT). This tool will ensure that the objects the user wishes to import are meeting more Elekta Synergy™ Dicom validation rule. The tool requires the user to manually validate an import.

In order to import a CT Image set, a RT Plan and a RT Structure set, these 3 different objects must be part of the same study and be linked by some Dicom Tags (see **Note XIV**). The RT Plan must contain an isocenter. The CT Image set must contain at least 2 images.

### 2.4.2 Association Establishment Policies

#### 2.4.2.1 General

The maximum PDU size for Elekta Synergy™ is configurable via initialisation file mergecom.pro from a minimum of 1024 bytes to a maximum of 31000 bytes. (The default is 16K = 16384 bytes).

#### 2.4.2.2 Number of Associations

Elekta Synergy™ will support one active association as a Service Class Provider at a time.

The number of simultaneous pending associations supported is configurable via initialisation file mergecom.pro. The default is 5.

### 2.4.2.3 Asynchronous Nature

Elekta Synergy™ does not support asynchronous operations and will not perform asynchronous operation negotiation.

### 2.4.2.4 Implementation Identifying Information

#### Release 3.5

The Implementation Class UID is: 1.3.46.423632.140000.3.5

The implementation version name is: XVI3.5

## 2.4.3 Association Initiation Policy

Elekta Synergy™ initiates associations as a result of the following local real-world activities:

- The operator requests export of one or more images from the local database to a remote application (see section 2.4.3.1)
- The operator queries a remote database (see section 2.4.3.2)
- The operator requests retrieval of one or more Dicom Object(RT Plan, RT Structure Set, CT Image, RT Image, SC Image) following querying of a remote database (see section 2.4.3.3)

### 2.4.3.1 Export Image(s) from Elekta Synergy™ to Remote Application

#### 2.4.3.1.1 Associated Real World Activity

The operator exports one or more images from the local Elekta Synergy™ database to a remote application by means of the Export function (accessed via the Elekta Synergy™ system user interface). After selecting the image(s) to be exported, and nominating the remote peer DICOM application entity, the operator confirms the image transfer request.

Elekta Synergy™ initiates one association to the selected peer and uses it to send the selected image(s) via C-STORE requests (and to receive the associated C-STORE Responses).

The association is released by Elekta Synergy™ after successful transfer of the image(s), or, in the event of transfer errors, when Elekta Synergy™ determines that too many errors have occurred.

#### 2.4.3.1.2 Proposed Presentation Contexts

Elekta Synergy™ will propose the following presentation contexts:

Table 3 Proposed Presentation Contexts for Elekta Synergy™ Import

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
SC Image Storage	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
RT Plan Storage	1.2.840.10008.5.1.4.1.1.48 1.5	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.48 1.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
RT Image Storage	1.2.840.10008.5.1.4.1.1.48 1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

#### 2.4.3.1.3 C-STORE SCU Conformance

While Elekta Synergy™ is busy transferring, the Busy status is displayed on the console and the user interface allows no interaction.

Elekta Synergy™ has the following behaviour upon successful and unsuccessful transfer of images:

- Success (return status 0000)

The user is notified of progress during transfer and normal control is returned upon completion of all transfers.

- Refused (return status A7xx) Error (return status A9xx or Cxxx) and Warning (return status B00x)

The user is notified that an (unspecified) error occurred whilst transferring an image. If the failure was specifically due to a Network error the user is additionally notified of this, and any outstanding transfers are cancelled immediately. For any other transfer failures, Elekta Synergy™ will attempt to continue transferring any remaining images in the selected set. If more than 5 transfer failures are reported during any export request the user is notified that too many errors have occurred, and any further outstanding transfers are cancelled.

APPENDIX A lists the applied DICOM attributes in the Secondary Capture IOD, RT Plan IOD, RT Structure Set IOD, RT Image IOD and CT Image IOD that are sent by Elekta Synergy™, and the mapping between these DICOM attributes and the Elekta Synergy™ database fields.

#### 2.4.3.2 Query a Remote Database

##### 2.4.3.2.1 Associated Real World Activity

The operator queries a remote database by means of the Patient DICOM Import function (accessed via the Elekta Synergy™ system user interface). The function permits the operator to browse the lists of patients held on remote applications and their corresponding Patient/Study/Series/Image hierarchies.

- Each time the operator selects a remote DICOM application and clicks the “query” button, Elekta Synergy™ initiates an association to the selected entity. It uses it to send a single C-FIND request for the list of filtered patients available on the remote system (and to receive the associated C-FIND responses). To filter the request the user can use the wildcard character, it replaces any substring. The association is released immediately by Elekta Synergy™ once all C-FIND responses have been received.
- Each time the operator selects a Patient, Study or Series from those presented as a result of a query, Elekta Synergy™ initiates a new association to the selected entity. This is used to send a single C-FIND request at the Level of Patient, Study, Series for the list of Studies, Series or Images available respectively (and to receive the associated C-FIND responses). The association is released immediately by Elekta Synergy™ once all C-FIND responses have been received.

#### 2.4.3.2.2 Proposed Presentation Contexts

Elekta Synergy™ will propose the following presentation contexts:

**Table 4 Proposed Presentation Contexts for Elekta Synergy™ Remote Database Query**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Patient Root Model Query/Retrieve FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

#### 2.4.3.2.3 C-FIND SCU Conformance

Elekta Synergy™ generates queries containing optional keys and displays the corresponding attributes from C-FIND responses into the user interface. If the remote application does not support optional keys (determined by service status Pending FF01) Elekta Synergy™ will silently ignore those attributes, displaying them as blank, and continue to receive responses.

The Required, Unique and Optional keys used in Elekta Synergy™ queries at the respective levels are listed below:

**Table 5 Patient Level Attributes used as Keys in C-FIND Queries**

Description	Tag	Type
Patients Name	(0010, 0010)	R
Patient ID	(0010, 0020)	U
Patient's Birth Date	(0010, 0030)	O
Patient's Sex	(0010, 0040)	O

**Table 6 Study Level Attributes used as Keys in C-FIND Queries**

Description	Tag	Type
Study Instance UID	(0020, 000D)	U
Study ID	(0020, 0010)	R
Study Date	(0008, 0020)	R
Study Time	(0008, 0030)	R
Accession Number	(0008, 0050)	R
Study Description	(0008, 1030)	O

**Table 7 Series Level Attributes used as Keys in C-FIND Queries**

Description	Tag	Type
Modality	(0008, 0060)	R
Series Instance UID	(0020, 000E)	U
Series Number	(0020, 0011)	R
Series Date	(0008, 0021)	O
Series Time	(0008, 0031)	O

**Table 8 Image Level Attributes used as Keys in C-FIND Queries**

Description	Tag	Type
Image Number	(0008, 0013)	R
SOP Instance UID	(0008, 0018)	U
Image Date	(0008, 0023)	O
Image Time	(0008, 0033)	O

### 2.4.3.3 Retrieve Image(s) from a Remote Database

#### 2.4.3.3.1 Associated Real World Activity

The operator retrieves one or more images from a remote application by means of the Patient DICOM Import function, having first performed a query on the remote database (as described in section 2.4.3.2). After selecting the image(s) from a selected Series to be imported, the operator confirms the Dicom object transfer request.

Elekta Synergy™ initiates one association to the selected peer and uses it to retrieve the selected Dicom object(s) via C-MOVE requests (and to receive the associated C-MOVE responses).

The association is released by Elekta Synergy™ after successful transfer of the Dicom object(s), or, in the event of transfer errors, when Elekta Synergy™ determines that too many errors have occurred.

The Dicom object(s) are stored into the Elekta Synergy™ DICOM Transit database as Dicom files (see section 2.4.1).

#### 2.4.3.3.2 Proposed Presentation Contexts

Elekta Synergy™ will propose the following presentation contexts:

**Table 9 Proposed Presentation Contexts for Elekta Synergy™ Remote Image Retrieve**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Patient Root Model Query/Retrieve MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

#### 2.4.3.3.3 C-MOVE SCU Conformance

The Elekta Synergy™ AE provides standard conformance.

C-MOVE requests are issued at the Image level for each Dicom object selected for retrieval.

## 2.4.4 Association Acceptance Policy

Elekta Synergy™ SCP Application Entity accepts associations for the following purposes:

- To allow remote applications to store Planning information and images into the Elekta Synergy™ Dicom Transit database (see section 2.4.4.1 below)
- To allow remote applications to verify application level communication with Elekta Synergy™ (see section 2.4.4.2 below)

Elekta Synergy™ may accept association requests from remote stations depending on Elekta Synergy™ configuration:

- The Application Entity rejects association requests that incorrectly address Elekta Synergy™ AE, i.e. from applications that offer a wrong “called AE title”. Elekta Synergy™ AE title is defined during configuration of the system (See Section 5.1.1).

### 2.4.4.1 Store RT data and Images into Elekta Synergy™ Database

#### 2.4.4.1.1 Associated Real World Activity

Elekta Synergy™ accepts associations from remote systems that wish to send images (RT Image, CT, SC Image) or RT data (RT Plan , RT Structure set) for storage into the Elekta Synergy™ database.

#### 2.4.4.1.2 Presentation Context Table

Any of the presentation contexts shown in

Table 10 and Table 11 are acceptable:

**Table 10      Acceptable Presentation Contexts for Elekta Synergy™ Non image Object Storage**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
RT Plan Storage - STORE	1.2.840.10008.5.1.4.1.1.481.5	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
RT Structure set Storage- STORE	1.2.840.10008.5.1.4.1.1.481.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 11. Acceptable Presentation contexts Elekta Synergy™ Image Storage

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
CT Image Storage - STORE	1.2.840.10008.5.1.4.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
SC Image Storage	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

#### 2.4.4.1.3 C-STORE SCP Conformance

Elekta Synergy™ provides standard conformance.

The AE is a Conformance Level 0 Storage SCP: not all DICOM Type 1 and 2 attributes are mapped in the database. However, no information is lost because we store the original Dicom message (except for SC Image) in the database and map only the attributes we are interested in. This should allow Elekta Synergy™ to make use of more Dicom attributes as its development progresses.

Incoming Dicom objects will be stored into a temporary database called Elekta Synergy™ Dicom Transit Database. (See 2.4.1)

APPENDIX A. specifies which attributes from the received RT Plan C-STORE requests are stored for internal Elekta Synergy™ use.

APPENDIX B. specifies which attributes from the received RT Structure Set C-STORE requests are stored for internal Elekta Synergy™ use.

APPENDIX C. specifies which attributes from the received CT Image C-STORE requests are stored for internal Elekta Synergy™ use and which attribute are u

APPENDIX B Explain the Extended Image Import Capability of Elekta Synergy™

APPENDIX C lists the specific C-STORE response status codes returned by the AE.

The duration of the storage of the RT Data and Images is determined by the operator of Elekta Synergy™.

#### 2.4.4.1.4 Presentation Context Acceptance Criterion

Elekta Synergy™ accepts all contexts in the intersection of the proposed and acceptable presentation contexts. There is no check for duplicate contexts. Duplicate contexts are accepted.

#### 2.4.4.1.5 Transfer Syntax Selection Policies

Elekta Synergy™ prefers its native byte ordering (Little Endian) , and will prefer explicit over implicit VR.

## 2.4.4.2 Verify Application Level Communication

### 2.4.4.2.1 Associated Real World Activity

Elekta Synergy™ accepts associations from systems that wish to verify the application level communication using the C-ECHO command.

### 2.4.4.2.2 Presentation Context Table

Any of the presentation contexts shown in Table 12 below are acceptable:

**Table 12 Acceptable Presentation Contexts for Verification**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

### 2.4.4.2.3 C-ECHO SCP Conformance

Elekta Synergy™ provides standard conformance.

### 2.4.4.2.4 Presentation Context Acceptance Criterion

Elekta Synergy™ accepts all contexts in the intersection of the proposed and acceptable presentation contexts. There is no check for duplicate contexts. Duplicate contexts are accepted.

### 2.4.4.2.5 Transfer Syntax Selection Policies

Elekta Synergy™ prefers its native byte ordering (Little Endian), and will prefer explicit over implicit VR.



## **3 Communication Profiles**

### **3.1 Supported Communication Stacks**

Elekta Synergy™ application provides DICOM V3.0 TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.

### **3.2 TCP/IP Stack**

Elekta Synergy™ inherits its TCP/IP stack from the Microsoft Windows XP (sp2) upon which it executes.

### **3.3 Physical Media Support**

Elekta Synergy™ supports Ethernet ISO.8802-3.

On Elekta supplied hardware platforms the connection type provided is 100/10BASE-T (RJ45 twisted pair).

## 4 Extensions/Specialisations/Privatisations

Not applicable.

## 5 Configuration

Elekta Synergy™ DICOM settings are configured by means of a DICOM-specific configuration program.

Configuration changes are effective immediately they are committed.

Configuration is intended to be performed by Elekta service engineers only.

### 5.1 AE Title/Presentation Address mapping

#### 5.1.1 Local AE Titles and Presentation Addresses

The local Application Entity Title is configurable via initialisation file sri.ini. The default is "Default"

The listen port number is configurable via the initialisation file mergecom.pro. The default is 104.

#### 5.1.2 Remote AE Titles and Presentation Addresses

All remote applications that wish to communicate with Elekta Synergy™ must be defined at Elekta Synergy™ DICOM configuration time.

The following information must be provided:

- The remote AE Title.
- The TCP/IP host name on which the remote application resides.
- The IP address of the remote host.
- The SOP classes for which the application provides conformance as an SCP.
- A user-readable alias string for identifying the remote application within the XVI user interface, (this string is presented to the operator when selecting a remote system, not the Remote AE Title.)

### 5.2 Configurable Parameters

#### 5.2.1 Communication Parameters

- The Maximum PDU size is configurable.
- The maximum number of simultaneous pending associations is configurable.
- The AE can be configured either to accept or reject association requests offering an unknown called AE title.
- Dicom Upper Layer Timeouts are configurable.

## 6 Support of Extended Character Sets

None.

## A. Applied RT Plan IOD and Mapping to Elekta Synergy™ Database

The modules selected from the RT Plan IOD of DICOM for prescription import are given in Table 13 below. If a module is not listed, none of the attributes in that module is stored by Elekta Synergy™.

**Table 13 Applied Modules in the RT Plan IOD for Import (SCP Role)**

IE	Module	Usage
Patient	Patient	M
Study	General Study	M
Series	RT Series (Ignored)	M
Plan	RT General Plan	M
	RT Patient Setup	U
	RT Fraction Scheme	M
	RT Beams	C
	Approval (Ignored)	U
	SOP Common	M

### A.1 RT Plan IOD Modules

Table 14 to Table 20 specify, for each of the applied modules above, the attributes stored by Elekta Synergy™, further details of mapping onto the Elekta Synergy™ database, and any attribute specific constraints applicable to their use.

Ignored attributes are not stored into the Elekta Synergy™ patient database. **However, all DICOM objects must conform to the DICOM standard.** If any part of a prescription does not conform to the standard then that prescription is not saved into the database and the storage request is rejected. Thus, Elekta Synergy™ performs validation of the entire applied IOD. I.e. where attributes irrelevant to Elekta Synergy™ are included in a message, they must still have values that are valid according to the DICOM standard. Storage requests containing invalid attributes will be REJECTED. (See Table 71, **Status Code A901**).

Table 14 RT Plan Storage SOP Class (SCP) – Patient Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Patients Name	(0010,0010)	PN 1	2	Split into Patient.first_name, Patient.last_name, Patient.mid_name (Prefix, Suffix not stored). See Note I , Note II
Patient ID	(0010, 0020)	LO 1	2	Patient.id See Note II
Patient's Birth Date	(0010, 0030)	DA 1	2	Patient.birth_date
Patients Sex	(0010, 0040)	CS 1	2	Patient.sex
Referenced Patient Sequence	(0008, 1120)	SQ 1	3	Ignored
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	
Patient's Birth Time	(0010, 0032)	TM 1	3	
Other Patient IDs	(0010, 1000)	LO 1-N	3	
Other Patient Names	(0010, 1001)	PN 1-N	3	
Ethnic Group	(0010, 2160)	SH 1	3	
Patient Comments	(0010, 4000)	LT 1	3	

**Note I Handling of Empty Patient Identification Attributes (RT Plan)**

The Patient ID (0010, 0020) and Patient Name (0010, 0010) attributes of the Patient Module are specified by DICOM as Type 2 and so may legally have zero length.

As a safety measure, however, **Elekta Synergy™** treats these attributes as Type 1 and will REJECT any RT Plan Storage request **containing** zero length values for these attributes. Which means these RT Plans won't enter the Elekta Synergy™ DICOM Transit database. (See **Table 71, Status Code C001**).

**Note II Patient ID Already Exists in Elekta Synergy™ Database (RT Plan)**

If a patient with the Patient ID specified in the RT Plan Storage request already exists in the Elekta Synergy™ Main database, no further Patient Module attributes in the request will be imported. The check for an existing Patient ID is insensitive to case or leading/trailing spaces.

Table 15 RT Plan Storage SOP Class (SCP) – General Study Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Study Instance UID	(0020, 000D)	UI 1	1	Treatment.dicom_uid see Note III
Study Date	(0008, 0020)	DA 1	2	Ignored
Study Time	(0008, 0030)	TM 1	2	
Referring Physicians Name	(0008, 0090)	PN 1	2	
Study ID	(0020, 0010)	SH 1	2	Treatment.id see Note III
Accession Number	(0008, 0050)	SH 1	2	
Study Description	(0008, 1030)	LO 1	3	Treatment.descrip see Note IV
Physician(s) of Record	(0008, 1048)	PN 1-N	3	Ignored
Name of Physician(s) Reading Study	(0008, 1060)	PN 1-N	3	
Referenced Study Sequence	(0008, 1110)	SQ 1	3	
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	

### Note III Handling of Empty Study ID Attribute and treatment creation

An incrementing counter is prepended to the treatment id then “:” and one of the following.

The applied Study ID (0020, 0010) is specified by DICOM as Type 2 and so may legally have zero length. This field is normally used by Elekta Synergy™ to identify the Treatment to be created or updated.

In the situation where the Study ID attribute is empty, Elekta Synergy™ will attempt to use the Accession Number (0008, 0050, Type 2) attribute as a Treatment ID instead. In such cases it will also append the Treatment Description with the text “: TRTID derived (Accession No.)” to assist the operator.

In the situation where both the Study ID and Accession Number attributes are empty, Elekta Synergy™ will use the last 16 digits of the Study Instance UID (0020, 000D) as a Treatment ID. In such cases it will also append the Treatment Description with the text “: TRTID derived (StudyInstanceUID.)” to assist the operator.

Extreme caution is advised when handling data with limited Study identification information present. It is the responsibility of the Elekta Synergy™ operator to ensure that incoming image data containing an empty Study ID attribute is correctly identified and qualified before relocation into the main Elekta Synergy™ Clinical database.

### Note IV Treatment Description

The treatment description is made of the Plan Name appended to the Study description appended to the Plan Label.

Table 16 RT Plan Storage SOP Class (SCP) – RT General Plan Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
RT Plan Label	(300A, 0002)	SH 1	1	Phase.name + appended to Phase.description
RT Plan Name	(300A, 0003)	LO 1	3	Treatment.name and Treatment.description created from RT Plan label + RT Plan name
RT Plan Description	(300A, 0004)	ST 1	3	Ignored
Operators Name	(0008, 1070)	PN 1-N	2	
RT Plan Date	(300A, 0006)	DA 1	2	
RT Plan Time	(300A, 0007)	TM 1	2	
Treatment Protocols	(300A, 0009)	LO 1-N	3	
Treatment Intent	(300A, 000A)	CS 1	3	
Treatment Sites	(300A, 000B)	LO 1-N	3	
RT Plan Geometry	(300A, 000C)	CS 1	1	
Referenced Structure Set Sequence	(300C, 0060)	SQ 1	1C	Used to link to RT Structure set ( see <b>Note XIV</b> )
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	Ignored
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	Used to link to RT Structure set ( see <b>Note XIV</b> )
Referenced Dose Sequence	(300C, 0080)	SQ 1	3	Ignored
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	
Referenced RT Plan Sequence	(300C, 0002)	SQ 1	3	
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	
>RT Plan Relationship	(300A, 0055)	CS 1	1C	



Table 17 RT Plan Storage SOP Class (SCP) – RT Patient Setup Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Patient Setup Sequence	(300A, 0180)	SQ 1	1	Ignored
>Patient Setup Number	(300A, 0182)	IS 1	1	
>Patient Position	(0018, 5100)	CS 1	1C	
>Patient Additional Position	(300A, 0184)	LO 1	1C	
>Fixation Device Sequence	(300A, 0190)	SQ 1	3	
>>Fixation Device Type	(300A, 0192)	CS 1	1C	
>>Fixation Device Label	(300A, 0194)	SH 1	2C	
>>Fixation Device Description	(300A, 0196)	ST 1	3	
>>Fixation Device Position	(300A, 0198)	SH 1	3	
>Shielding Device Sequence	(300A, 01A0)	SQ 1	3	
>>Shielding Device Type	(300A, 01A2)	CS 1	1C	
>>Shielding Device Label	(300A, 01A4)	SH 1	2C	
>>Shielding Device Description	(300A, 01A6)	ST 1	3	
>>Shielding Device Position	(300A, 01A8)	SH 1	3	
>Setup Technique	(300A, 01B0)	CS 1	3	
>Setup Technique Description	(300A, 01B2)	ST 1	3	
>Setup Device Sequence	(300A, 01B4)	SQ 1	3	
>>Setup Device Type	(300A, 01B6)	CS 1	1C	
>>Setup Device Label	(300A, 01B8)	SH 1	2C	
>>Setup Device Description	(300A, 01BA)	ST 1	3	
>>Setup Device Parameter	(300A, 01BC)	DS 1	2C	
>>Setup Reference Description	(300A, 01D0)	ST 1	3	
>Table Top Vertical Setup Displacement	(300A, 01D2)	DS 1	3	Can be used for import validation. See <b>Note V Import validation</b>
>Table Top Longitudinal Setup Displacement	(300A, 01D4)	DS 1	3	
>Table Top Lateral Setup Displacement	(300A, 01D6)	DS 1	3	

**Note V Import validation**

The validation of a Dicom import into the main database has 3 different modes configurable via the sri.ini file.

1. Isocenter validation: the user is asked to enter the isocenter defined in the plan he is about to import.
2. Patient setup table displacement validation : the user is asked to enter the Table top vertical, longitudinal, lateral setup
3. No validation.

In all cases the user is warned about the implication of importing a wrong plan and is presented with extra information about the plan and asked a confirmation.

Table 18 RT Plan Storage SOP Class (SCP) – RT Fraction Scheme Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Fraction Group Sequence	(300A, 0070)	SQ 1	1	
>Fraction Group Number	(300A, 0071)	IS 1	1	Fraction.ID
>Referenced Patient Setup Number	(300C, 006A)	IS 1	3	Ignored
>Referenced Dose Sequence	(300C, 0080)	SQ 1	3	
>>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	
>Referenced Dose Reference Sequence	(300C, 0050)	SQ 1	3	
>>Referenced Dose Reference Number	(300C, 0051)	IS 1	1C	
>>Constraint Weight	(300A, 0021)	DS 1	3	
>>Delivery Warning Dose	(300A, 0022)	DS 1	3	
>>Delivery Maximum Dose	(300A, 0023)	DS 1	3	
>>Target Minimum Dose	(300A, 0025)	DS 1	3	
>>Target Prescription Dose	(300A, 0026)	DS 1	3	
>>Target Maximum Dose	(300A, 0027)	DS 1	3	
>>Target Underdose Volume Fraction	(300A, 0028)	DS 1	3	
>>Organ at Risk Full-volume Dose	(300A, 002A)	DS 1	3	
>>Organ at Risk Limit Dose	(300A, 002B)	DS 1	3	
>>Organ at Risk Maximum Dose	(300A, 002C)	DS 1	3	
>>Organ at Risk Overdose Volume Fraction	(300A, 002D)	DS 1	3	
>Number of Fractions Planned	(300A, 0078)	IS 1	2	
>Number of Fractions Per Day	(300A, 0079)	IS 1	3	
>Repeat Fraction Cycle Length	(300A, 007A)	IS 1	3	
>Fraction Pattern	(300A, 007B)	LT 1	3	
>Number of Beams	(300A, 0080)	IS 1	1	
>Referenced Beam Sequence	(300C, 0004)	SQ 1	1C	
>>Referenced Beam Number	(300C, 0006)	IS 1	1C	
>>Beam Dose Specification Point	(300A, 0082)	DS 3	3	
>>Beam Dose	(300A, 0084)	DS 1	3	
>>Beam Meterset	(300A, 0086)	DS 1	3	
>Number of Brachy Application Setups	(300A, 00A0)	IS 1	1	
>Referenced Brachy Application Setup Sequence	(300C, 000A)	SQ 1	1C	
>>Referenced Brachy Application Setup Number	(300C, 000C)	IS 1	1C	
>>Brachy Application Setup Dose Specification Point	(300A, 00A2)	DS 3	3	
>>Brachy Application Setup Dose	(300A, 00A4)	DS 1	3	

**Table 19 RT Plan Storage SOP Class (SCP) – RT Beams Module**

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Beam Sequence	(300A, 00B0)	SQ 1	1	
>Beam Number	(300A, 00C0)	IS 1	1	Field.beam_number
>Beam Name	(300A, 00C2)	LO, 1	3	Field.ID (combined Beam Number and Name) Field.beam_name
>Beam Description	(300A, 00C3)	ST 1	3	Field.description
>Beam Type	(300A, 00C4)	CS 1	1	Ignored
>Radiation Type	(300A, 00C6)	CS 1	2	
>Treatment Machine Name	(300A, 00B2)	SH 1	2	
>Manufacturer	(0008, 0070)	LO 1	3	
>Institution Name	(0008, 0080)	LO 1	3	
>Institution Address	(0008, 0081)	ST 1	3	
>Institutional Department Name	(0008, 1040)	LO 1	3	
>Manufacturers Model Name	(0008, 1090)	LO 1	3	
>Device Serial Number	(0018, 1000)	LO 1	3	
>Primary Dosimeter Unit	(300A, 00B3)	CS 1	3	
>Referenced Tolerance Table Number	(300C, 00A0)	IS 1	3	
>Source-Axis Distance	(300A, 00B4)	DS 1	3	
>Beam Limiting Device Sequence	(300A, 00B6)	SQ 1	1	
>>RT Beam Limiting Device Type	(300A, 00B8)	CS 1	1	
>>Source to Beam Limiting Device Distance	(300A, 00BA)	DS 1	3	
>>Number of Leaf/Jaw Pairs	(300A, 00BC)	IS 1	1	
>>Leaf Position Boundaries	(300A, 00BE)	DS 3-N	2C	
>Referenced Patient Setup Number	(300C, 006A)	IS 1	3	
>Referenced Reference Image Sequence	(300C, 0042)	SQ 1	3	
>>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	
>>Reference Image Number	(300A, 00C8)	IS 1	1C	
>>Start Cumulative Meterset Weight	(300C, 0008)	DS 1	3	
>>End Cumulative Meterset Weight	(300C, 0009)	DS 1	3	
>Planned Verification Image Sequence	(300A, 00CA)	SQ 1	3	
>>Start Cumulative Meterset Weight	(300C, 0008)	DS 1	3	
>>Meterset Exposure	(3002, 0032)	DS 1	3	
>>End Cumulative Meterset Weight	(300C, 0009)	DS 1	3	
>>RT Image Plane	(3002, 000C)	CS 1	3	
>>X-Ray Image receptor Angle	(3002, 000E)	DS 1	3	
>>RT Image Orientation	(3002, 0010)	DS 6	3	
>>RT Image Position	(3002, 0012)	DS 2	3	
>>RT Image SID	(3002, 0026)	DS 1	3	
>>Imaging Device-Specific Acquisition Parameters	(300A, 00CC)	LO 1-N	3	

>>Referenced Reference Image Number	(300C, 0007)	IS 1	3
>Treatment Delivery Type	(300A, 00CE)	CS 1	3
>Referenced Dose Sequence	(300C, 0080)	SQ 1	3
>>Referenced SOP Class UID	(0008, 1150)	UI 1	1C
>>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C
>Number of Wedges	(300A, 00D0)	IS 1	1
>Wedge Sequence	(300A, 00D1)	SQ 1	1C
>>Wedge Number	(300A, 00D2)	IS 1	1C
>>Wedge Type	(300A, 00D3)	CS 1	2C
>>Wedge ID	(300A, 00D4)	SH 1	3
>>Wedge Angle	(300A, 00D5)	IS 1	2C
>>Wedge Factor	(300A, 00D6)	DS 1	2C
>>Wedge Orientation	(300A, 00D8)	DS 1	2C
>>Source to Wedge Tray Distance	(300A, 00DA)	DS 1	3
>Number of Compensators	(300A, 00E0)	IS 1	1
>Total Compensator Tray Factor	(300A, 00E2)	DS 1	3
>Compensator Sequence	(300A, 00E3)	SQ 1	1C
>>Compensator Number	(300A, 00E4)	IS 1	1C
>>Material ID	(300A, 00E1)	SH 1	2C
>>Compensator ID	(300A, 00E5)	SH 1	3
>>Source to Compensator Tray Distance	(300A, 00E6)	DS 1	2C
>>Compensator Rows	(300A, 00E7)	IS 1	1C
>>Compensator Columns	(300A, 00E8)	IS 1	1C
>>Compensator Pixel Spacing	(300A, 00E9)	DS 2	1C
>>Compensator Position	(300A, 00EA)	DS 2	1C
>>Compensator Transmission Data	(300A, 00EB)	DS 1-N	1C
>>Compensator Thickness Data	(300A, 00EC)	DS 1-N	1C
>Number of Boli	(300A, 00ED)	IS 1	1
>Referenced Bolus Sequence	(300C, 00B0)	SQ 1	1C
>>Referenced ROI Number	(3006, 0084)	IS 1	1C
>Number of Blocks	(300A, 00F0)	IS 1	1
>Total Block Tray Factor	(300A, 00F2)	DS 1	3
>Block Sequence	(300A, 00F4)	SQ 1	1C
>>Block Tray ID	(300A, 00F5)	SH 1	3
>>Source to Block Tray Distance	(300A, 00F6)	DS 1	2C
>>Block Type	(300A, 00F8)	CS 1	1C
>>Block Divergence	(300A, 00FA)	CS 1	2C
>>Block Number	(300A, 00FC)	IS 1	1C
>>Block Name	(300A, 00FE)	LO 1	3
>>Material ID	(300A, 00E1)	SH 1	2C
>>Block Thickness	(300A, 0100)	DS 1	2C
>>Block Transmission	(300A, 0102)	DS 1	2C
>>Block Number of Points	(300A, 0104)	IS 1	2C
>>Block Data	(300A, 0106)	DS 2-2N	2C
>Applicator Sequence	(300A, 0107)	SQ 1	3
>>Applicator ID	(300A, 0108)	SH 1	1C
>>Applicator Type	(300A, 0109)	CS 1	1C
>>Applicator Description	(300A, 010A)	LO 1	3
>Final Cumulative Meterset Weight	(300A, 010E)	DS 1	1C

>Number of Control Points	(300A, 0110)	IS 1	1	
>Control Point Sequence	(300A, 0111)	SQ 1	1	
>>Control Point Index	(300A, 0112)	IS 1	1C	
>>Block Thickness	(300A, 0100)	DS 1	2C	
>>Block Transmission	(300A, 0102)	DS 1	2C	
>>Block Number of Points	(300A, 0104)	IS 1	2C	
>>Block Data	(300A, 0106)	DS 2-2N	2C	
>Applicator Sequence	(300A, 0107)	SQ 1	3	
>>Applicator ID	(300A, 0108)	SH 1	1C	
>>Applicator Type	(300A, 0109)	CS 1	1C	
>>Applicator Description	(300A, 010A)	LO 1	3	
>Final Cumulative Meterset Weight	(300A, 010E)	DS 1	1C	
>Number of Control Points	(300A, 0110)	IS 1	1	
>Control Point Sequence	(300A, 0111)	SQ 1	1	
>>Control Point Index	(300A, 0112)	IS 1	1C	
>>Cumulative Meterset Weight	(300A, 0134)	DS 1	2C	Field.total_dose (used the 1 <sup>st</sup> control point of the sequence)
>>Referenced Dose Reference Sequence	(300C, 0050)	SQ 1	3	Ignored
>>>Referenced Dose Reference Number	(300C, 0051)	IS 1	1C	
>>>Cumulative Dose Reference Coefficient	(300A, 010C)	DS 1	2C	
>>Nominal Beam Energy	(300A, 0114)	DS 1	3	Field.energy (used the 1 <sup>st</sup> control point of the sequence)
>>Dose Rate Set	(300A, 0115)	DS 1	3	Field.dose_rate (used the 1 <sup>st</sup> control point of the sequence)
>>Wedge Position Sequence	(300A, 0116)	SQ 1	3	Ignored
>>Wedge Position Sequence	(300A, 0116)	SQ 1	3	
>>>Referenced Wedge Number	(300C, 00C0)	IS 1	1C	
>>>Wedge Position	(300A, 0118)	CS 1	1C	
>>Beam Limiting Device Position Sequence	(300A, 011A)	SQ 1	1C	
>>>RT Beam Limiting Device Type	(300A, 00B8)	CS 1	1C	
>>>Leaf/Jaw Positions	(300A, 011C)	DS 2-2N	1C	
>>Gantry Angle	(300A, 011E)	DS 1	1C	Field.gantry_angle (used the 1 <sup>st</sup> control point of the sequence)
>>Gantry Rotation Direction	(300A, 011F)	CS 1	1C	Ignored
>>Beam Limiting Device Angle	(300A, 0120)	DS 1	1C	
>>Beam Limiting Device Rotation Direction	(300A, 0121)	CS 1	1C	
>>Patient Support Angle	(300A, 0122)	DS 1	1C	
>>Patient Support Rotation Direction	(300A, 0123)	CS 1	1C	
>>Table Top Eccentric Axis Distance	(300A, 0124)	DS 1	3	
>>Table Top Eccentric Angle	(300A, 0125)	DS 1	1C	
>>Table Top Eccentric Rotation Direction	(300A, 0126)	CS 1	1C	
>>Table Top Vertical Position	(300A, 0128)	DS 1	2C	
>>Table Top Longitudinal Position	(300A, 0129)	DS 1	2C	
>>Table Top Lateral Position	(300A, 012A)	DS 1	2C	

>>Isocenter Position	(300A, 012C)	DS 3	2C	Split into Isocenter.x , Isocenter.y , Isocenter.z DIVT: These values will be checked against user input if DIVT uses Isocenter as Plan Validation method. See <b>Note V Import validation</b>
>>Surface Entry Point	(300A, 012E)	DS 3	3	
>>Source to Surface Distance	(300A, 0130)	DS 1	3	Field.ssd (used the 1 <sup>st</sup> control point of the sequence)

**Table 20 RT Plan Storage SOP Class (SCP) – SOP Common Module**

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
SOP Class UID	(0008, 0016)	UI 1	1	
SOP Instance UID	(0008, 0018)	UI 1	1	RTPlan.dicom_uid
Specific Character Set	(0008, 0005)	CS 1-N	1C	
Instance Creation Date	(0008, 0012)	DA 1	3	
Instance Creation Time	(0008, 0013)	TM 1	3	
Instance Creator UID	(0008, 0014)	UI 1	3	

## B. Applied RT Structure Set IOD and mapping to Elekta Synergy™ Database

### B.1 Import of RT Structure Set

The modules selected from the RT Structure Set IOD of DICOM for prescription import are given in Table 21. If a module is not listed, none of the attributes in that module is stored by Elekta Synergy™.

**Table 21 Applied Modules in the RT Structure Set IOD for Import (SCP Role)**

IE	Module	Usage
Patient	Patient	M
Study	General Study (Ignored)	M
Series	RT Series (Ignored)	M
Equipment	General Equipment (Ignored)	M
Structure Set	Structure set	M
	ROI contour	M
	ROI Observation (Ignored)	M
	SOP Common	M

### B.2 RT Structure Set IOD Modules

Table 22 to Table 25 specify, for each of the applied modules above, the attributes stored by Elekta Synergy™, further details of mapping onto the Elekta Synergy™ database, and any attribute specific constraints applicable to their use.

Ignored attributes are not stored into the Elekta Synergy™ patient database. **However, all DICOM objects must conform to the DICOM standard.** If any part of a RT Structure Set does not conform to the standard then that prescription is not saved into the database and the storage request is rejected. Thus, Elekta Synergy™ performs validation of the entire applied IOD. I.e. where attributes irrelevant to Elekta Synergy™ are included in a message, they must still have values that are valid according to the DICOM standard. Storage requests containing invalid attributes will be REJECTED. (See Table 71, **Status Code A901**).



Table 22 RT Structure Set Storage SOP Class (SCP) – Patient Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Patients Name	(0010,0010)	PN 1	2	See Note VI
Patient ID	(0010, 0020)	LO 1	2	See Note VII
Patient's Birth Date	(0010, 0030)	DA 1	2	Ignored
Patients Sex	(0010, 0040)	CS 1	2	
Referenced Patient Sequence	(0008, 1120)	SQ 1	3	
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	
Patient's Birth Time	(0010, 0032)	TM 1	3	
Other Patient IDs	(0010, 1000)	LO 1-N	3	
Other Patient Names	(0010, 1001)	PN 1-N	3	
Ethnic Group	(0010, 2160)	SH 1	3	
Patient Comments	(0010, 4000)	LT 1	3	

**Note VI Handling of Empty Patient Identification Attributes**

The Patient ID (0010, 0020) and Patient Name (0010, 0010) attributes of the Patient Module are specified by DICOM as Type 2 and so may legally have zero length.

As a safety measure, however, **Elekta Synergy™** treats these attributes as Type 1 and will REJECT any RT Structure Set Storage request containing zero length values for these attributes. Which means this RT Structure Set won't enter the Elekta Synergy™ DICOM Transit database. (See **Table 71, Status Code C001**).

**Note VII Patient ID Already Exists in Elekta Synergy™ Database**

If a patient with the Patient ID specified in the RT Structure Set Storage request already exists in the Elekta Synergy™ Main database, no further Patient Module attributes in the request will be imported. The check for an existing Patient ID is insensitive to case or leading/trailing spaces.

**Note VIII Mapping in Main database**

The values of this module are not used directly to populate a patient record in the main database because a RT Structure set is always imported with a RT Plan and at least 2 Ct images. Nonetheless the Elekta Synergy™ SCP performs the same checks on Patient ID and Patient name, and an error on one these would result in a transfer failure to our Elekta Synergy™ DICOM Transit database.

Table 23 RT Structure Set Storage SOP Class (SCP) – ROI contour Module

Attribute Name	Tag	VR, VM	DICOM M Type	Notes/Constraints
ROI Contour Sequence	(3006,0039)	SQ	1	See <b>Note IX</b>
>Referenced ROI Number	(3006,0084)	IS 1	1	See <b>Note IX</b>
>ROI Display Color	(3006,002A)	IS 3	3	See <b>Note IX</b> (used to create LUT table)
>Contour Sequence	(3006,0040)	SQ 1	3	See <b>Note IX</b>
>>Contour Number	(3006,0048)	IS 1	3	See <b>Note IX</b>
>>Attached Contours	(3006,0049)	IS 1-n	3	Ignored
>>Contour Image Sequence	(3006,0016)	SQ 1	3	
>>>Referenced SOP Class UID	(0008,1150)	UI 1	1C	
>>>Referenced SOP Instance UID	(0008,1155)	UI 1	1C	
>>>Referenced Frame Number	(0008,1160)	IS 1-n	1C	
>>Contour Geometric Type	(3006,0042)	CS 1	1C	See <b>Note IX</b>
>>Contour Slab Thickness	(3006,0044)	DS 1	3	Ignored
>>Contour Offset Vector	(3006,0045)	DS 3	3	
>>Number of Contour Points	(3006,0046)	IS 1	1C	See <b>Note IX</b>
>>Contour Data	(3006,0050)	DS 3-3n	1C	See <b>Note IX</b>

Table 24 RT Structure Set SOP Class (SCP) – Structure Set Module

Attribute Name	Tag	VR, VM	Type	Description
Structure Set Label	(3006,0002)	SH 1	1	Ignored
Structure Set Name	(3006,0004)	LO 1	3	
Structure Set Description	(3006,0006)	ST 1	3	
Instance Number	(0020,0013)	IS 1	3	
Structure Set Date	(3006,0008)	DA 1	2	
Referenced Frame of Reference Sequence	(3006,0010)	SQ 1	3	
>Frame of Reference UID	(0020,0052)	UI 1	1C	Used to link to CT Images (see <b>Note XIV</b> )
>Frame of Reference Relationship Sequence	(3006,00C0)	SQ 1	3	Ignored
>>Related Frame of Reference UID	(3006,00C2)	UI 1	1C	
>>Frame of Reference Transformation Type	(3006,00C4)	CS 1	1C	
>>Frame of Reference Transformation Matrix	(3006,00C6)	DS 16	1C	
>>Frame of Reference Transformation Comment	(3006,00C8)	LO 1	3	
>RT Referenced Study Sequence	(3006,0012)	SQ 1	3	
>>Referenced SOP Class UID	(0008,1150)	UI 1	1C	
>>Referenced SOP Instance UID	(0008,1155)	UI 1	1C	
>>RT Referenced Series Sequence	(3006,0014)	SQ 1	1C	
>>>Series Instance UID	(0020,000E)	UI 1	1C	
>>>Contour Image Sequence	(3006,0016)	SQ 1	1C	
>>>>Referenced SOP Class UID	(0008,1150)	UI 1	1C	
>>>>Referenced SOP Instance UID	(0008,1155)	UI 1	1C	
>>>>Referenced Frame Number	(0008,1160)	IS 1-n	3	
Structure Set ROI Sequence	(3006,0020)	SQ 1	3	
>ROI Number	(3006,0022)	IS 1	1C	
>Referenced Frame of Reference UID	(3006,0024)	UI 1	1C	Ignored
>ROI Name	(3006,0026)	LO 1	2C	See <b>Note IX</b> (used to create LUT table)
>ROI Description	(3006,0028)	ST 1	3	Ignored
>ROI Volume	(3006,002C)	DS 1	3	
>ROI Generation Algorithm	(3006,0036)	CS 1	2C	
>ROI Generation Description	(3006,0038)	LO 1	3	

**Note IX Useful attribute not saved in database:**

These attributes are used in processing a visualisation file compatible with XVI viewer during import from the Elekta Synergy™ DICOM Transit database to the main database.

Table 25 RT Structure Set Storage SOP Class (SCP) – SOP Common Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
SOP Class UID	(0008,0016)	UI 1	1	Ignored
SOP Instance UID	(0008,0018)	UI 1	1	StructureSet.dicom_uid, used to link to RT Plans. (see <b>Note XIV</b> )
Specific Character Set	(0008,0005)	CS 1-N	1C	Ignored
Instance Creation Date	(0008,0012)	DA 1	3	
Instance Creation Time	(0008,0013)	TM 1	3	
Instance Creator UID	(0008,0014)	UI 1	3	

## C. Applied CT Image IOD and mapping to Elekta Synergy™ Database

### C.1 Import of CT Image

The modules selected from the CT Image IOD of DICOM for prescription import are given in Table 26. If a module is not listed, none of the attributes in that module is stored by Elekta Synergy™.

Table 26 Applied Modules in the CT Image IOD for Import (SCP Role)

IE	MODULE	USAGE
Patient	Patient	M
Study	General Study (Ignored)	M
Series	General Series	M
Frame of reference	Frame of Reference	M
Equipment	General equipment (Ignored)	M
Image	General image (Ignored)	M
	Image plane	M
	Image Pixel	M
	CT Image	M
	SOP Common (Ignored)	M

Table 27 to Table 28 specify, for each of the applied modules above, the attributes stored by Elekta Synergy™, further details of mapping onto the Elekta Synergy™ database, and any attribute specific constraints applicable to their use.

Ignored attributes are not stored into the Elekta Synergy™ patient database. **However, all DICOM objects must conform to the DICOM standard.** If any part of a CT Image does not conform to the standard then that prescription is not saved into the database and the storage request is rejected. Thus, Elekta Synergy™ performs validation of the entire applied IOD. I.e. where attributes irrelevant to Elekta Synergy™ are included in a message, they must still have values that are valid according to the DICOM standard. Storage requests containing invalid attributes will be REJECTED. (See Table 71, Status Code A901).

Table 27 CT Image Storage SOP Class (SCP) – Patient Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Patients Name	(0010,0010)	PN 1	2	See Note X and Note XI
Patient ID	(0010, 0020)	LO 1	2	See Note X and Note XI
Patient's Birth Date	(0010, 0030)	DA 1	2	Ignored
Patients Sex	(0010, 0040)	CS 1	2	
Referenced Patient Sequence	(0008, 1120)	SQ 1	3	
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	
Patient's Birth Time	(0010, 0032)	TM 1	3	
Other Patient IDs	(0010, 1000)	LO 1-N	3	
Other Patient Names	(0010, 1001)	PN 1-N	3	
Ethnic Group	(0010, 2160)	SH 1	3	
Patient Comments	(0010, 4000)	LT 1	3	

**Note X Handling of Empty Patient Identification Attributes**

The Patient ID (0010, 0020) and Patient Name (0010, 0010) attributes of the Patient Module **are** specified by DICOM as Type 2 and so may legally have zero length.

As a safety measure, however, **Elekta Synergy™** treats these attributes as Type 1 and will REJECT any RT Plan Storage request containing zero length values for these attributes. (See **Table 71, Status Code C001**).

**Note XI Patient ID Already Exists in Elekta Synergy™ Database**

If a patient with the Patient ID specified in the CT Image Storage request already exists in the Elekta Synergy™ database, no further Patient Module attributes in the request will be imported. The check for an existing Patient ID is insensitive to case or leading/trailing spaces.

**Note XII Mapping in Main database**

The values of this module are not used directly to populate a patient record in the main database because a CT Image is always imported with a RT Plan and a RT Structure set. Nonetheless the Elekta Synergy™ SCP performs the same checks on Patient ID and Patient name, and an error on one of these would result in a transfer failure to our Elekta Synergy™ DICOM Transit Database.

**Table 28 CT Image SOP Class (SCP) – General Series Module**

Name	Tag	Type	VR , VM	Notes/Constraints	
Modality	(0008,0060)	1	CS 1	Ignored	
Series Instance UID	(0020,000E)	1	UI 1	CT.dicom_uid	
Series Number	(0020,0011)	2	IS 1	Ignored	
Series Date	(0008,0021)	3	DA 1		
Series Time	(0008,0031)	3	TM 1		
Performing Physicians' Name	(0008,1050)	3	PN 1-n		
Performing Physician Identification Sequence	(0008,1052)	3	SQ 1		
Protocol Name	(0018,1030)	3	LO 1		
Series Description	(0008,103E)	3	LO 1		
Operators' Name	(0008,1070)	3	PN 1-n		
Operator Identification Sequence	(0008,1072)	3	SQ 1		
Referenced Performed Procedure Step Sequence	(0008,1111)	3	SQ 1		
>Referenced SOP Class UID	(0008,1150)	1C	UI 1		
>Referenced SOP Instance UID	(0008,1155)	1C	UI 1		
Body Part Examined	(0018,0015)	3	CS 1		
Patient Position	(0018,5100)	2C	CS 1		Used for viewer file creation(Note IX )
Smallest Pixel Value in Series	(0028,0108)	3	US or SS 1		Ignored
Largest Pixel Value in Series	(0028,0109)	3	US or SS 1		
Request Attributes Sequence	(0040,0275)	3	SQ 1		
>Requested Procedure ID	(0040,1001)	1C	SH 1		
>Scheduled Procedure Step ID	(0040,0009)	1C	SH 1		
>Scheduled Procedure Step Description	(0040,0007)	3	LO 1		
>Scheduled Protocol Code Sequence	(0040,0008)	3	SQ 1		
Performed Procedure Step ID	(0040,0253)	3	SH 1		
Performed Procedure Step Start Date	(0040,0244)	3	DA 1		
Performed Procedure Step Start Time	(0040,0245)	3	TM 1		
Performed Procedure Step Description	(0040,0254)	3	LO 1		

Performed Protocol Code Sequence	(0040,0260)	3	SQ 1	
Comments on the Performed Procedure Step	(0040,0280)	3	ST 1	

**Note XIII Tags used but stored in Dicom file**


All other tables are ignored as far as the database is concerned. However the Dicom file is saved and is loaded and processed every time it has to be displayed.

**Table 29 CT Image Storage SOP Class (SCP) – Frame of reference Module**

Name	Tag	VR, VM	Type	Notes/Constraints
Frame of reference UID	(0020,0052)	UI 1	1	Used to link to Structure set (see <b>Note XIV</b> )
Position Reference Indicator	(0020,1040)	LO 1	2	Ignored

**Note XIV Linking of Dicom objects:**

Elekta Synergy only allows import of CT Image, RT Structure set or RT Plan from the Elekta Synergy Dicom Transit database to the main database (Using the interface DIVT) if they are part of a complete Dicom set. The relation between these objects is detected by checking the values of specific tags (see Figure 2)

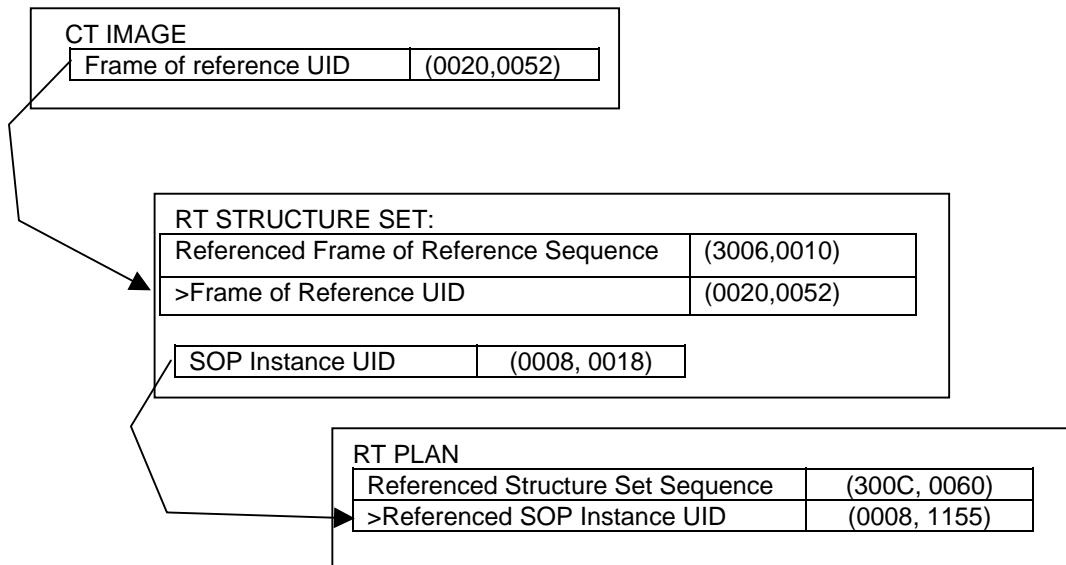

**Figure 2 Tags used to link Dicom set**

Table 30 CT Image Storage SOP Class (SCP) –Image Plane Module

Name	Tag	DICOM Type	VM, VR	Notes/Constraints
Pixel spacing	(0028,0030)	1	DS 2	Used for viewer file creation( <b>Note IX</b> )
Image Orientation (Patient)	(0020,0037)	1	DS 6	Used for viewer file creation( <b>Note IX</b> )
Image Position (Patient)	(0020,0032)	1	DS 3	Used for viewer file creation( <b>Note IX</b> )
Slice Thickness	(0018,0050)	1	DS 1	Used for viewer file creation( <b>Note IX</b> )
Slice Location	(0020,1041)	3	DS 1	Ignored

Table 31 CT Image Storage SOP Class (SCP) –Image Pixel Module

Name	Tag	DICOM Type	VM, VR	Notes/Constraints
Samples per Pixel	(0028,0002)	1	US 1	
Photometric Interpretation	(0028,0004)	1	CS 1	
Rows	(0028,0010)	1	US 1	Used for viewer file creation( <b>Note IX</b> )
Columns	(0028,0011)	1	US 1	Used for viewer file creation( <b>Note IX</b> )
Bits Allocated	(0028,0100)	1	US 1	Used for viewer file creation( <b>Note IX</b> ) (see Note XV)
Bits Stored	(0028,0101)	1	US 1	Used for viewer file creation( <b>Note IX</b> )
High Bit	(0028,0102)	1	US 1	
Pixel Representation	(0028,0103)	1	US 1	Used for viewer file creation( <b>Note IX</b> )
Pixel Data	(7FE0,0010)	1	OW or OB 1	Used for viewer file creation( <b>Note IX</b> )
Planar Configuration	(0028,0006)	1C	US 1	
Pixel Aspect Ratio	(0028,0034)	1C	IS 2	
Smallest Image Pixel Value	(0028,0106)	3	US or SS 1	
Largest Image Pixel Value	(0028,0107)	3	US or SS 1	
Red Palette Color Lookup Table Descriptor	(0028,1101)	1C	US or SS 3	
Green Palette Color Lookup Table Descriptor	(0028,1102)	1C	US or SS 3	
Blue Palette Color Lookup Table Descriptor	(0028,1103)	1C	US or SS 3	
Red Palette Color Lookup Table Data	(0028,1201)	1C	OW 1	
Green Palette Color Lookup Table Data	(0028,1202)	1C	OW 1	
Blue Palette Color Lookup Table Data	(0028,1203)	1C	OW 1	

**Note XV handling of non 16 bit CT Images**

We will reject the non 16 bit images, the check will be made against the Bits allocated tag (0028,0100) from the CT Image module (**Status Code C028**)

Table 32 CT Image Storage SOP Class (SCP) –CT Image Module

Name	Tag	DICOM	VM, VR	Notes/Constraints
------	-----	-------	--------	-------------------



Type				
Image Type	(0008,0008)	1	CS 1-n	Ignored
Samples per Pixel	(0028,0002)	1	US 1	
Photometric Interpretation	(0028,0004)	1	CS 1	
Bits Allocated	(0028,0100)	1	US 1	
Bits Stored	(0028,0101)	1	US 1	Used for viewer file creation(Note <b>IX</b>
High Bit	(0028,0102)	1	US 1	Ignored
Rescale Intercept	(0028,1052)	1	DS 1	Used for viewer file creation(Note <b>IX</b> )
Rescale Slope	(0028,1053)	1	DS 1	Used for viewer file creation(Note <b>IX</b> )
KVP	(0018,0060)	2	DS 1	Ignored
Acquisition Number	(0020,0012)	2	IS 1	
Scan Options	(0018,0022)	3	CS 1-n	
Data Collection Diameter	(0018,0090)	3	DS 1	
Reconstruction Diameter	(0018,1100)	3	DS 1	
Distance Source to Detector	(0018,1110)	3	DS 1	
Distance Source to Patient	(0018,1111)	3	DS 1	
Gantry/Detector Tilt	(0018,1120)	3	DS 1	
Table Height	(0018,1130)	3	DS 1	
Rotation Direction	(0018,1140)	3	CS 1	
Exposure Time	(0018,1150)	3	IS 1	
X-ray Tube Current	(0018,1151)	3	IS 1	
Exposure	(0018,1152)	3	IS 1	
Exposure in $\mu$ As	(0018,1153)	3	IS 1	
Filter Type	(0018,1160)	3	SH 1	
Generator Power	(0018,1170)	3	IS 1	
Focal Spot	(0018,1190)	3	DS 1-n	
Convolution Kernel	(0018,1210)	3	DS 1	

## C.2 Export of CT Image

The modules selected from the CT Image IOD table of DICOM for image export are given in Table 59 below. If a module is not listed, none of the attributes in that module is sent by Elekta Synergy™.

**Table 33 Applied Modules in the CT Image IOD for Import (SCU Role)**

IE	MODULE	USAGE
Patient	Patient	M
Study	General Study	M
Series	General Series	M
Frame of reference	Frame of Reference	M
Equipment	General equipment	M
Image	General image	M
	Image plane	M
	Image Pixel	M
	CT Image	M
	SOP Common	M

Table 60 to Table 68 below specify the applied attributes for each module, and note their mappings from the Elekta Synergy™ database. If an attribute is not listed it is not sent by Elekta Synergy™. If an attribute is listed without Notes, there is a mapping from a directly equivalent Elekta Synergy™ database entry. Only the tags populated are listed.

**Table 34 CT Image Storage SOP Class (SCU) – Patient Module**

Attribute Name	Tag	DICOM Type	VM, VR	Notes
Patients Name	(0010,0010)	2	PN 1	Patient.Last^ Patient.First^ Patient.Middle^^ (no Prefix or Suffix)
Patient ID	(0010, 0020)	2	LO 1	Patient.ID
Patient's Birth Date	(0010, 0030)	2	DA 1	Patient.birth_date
Patients Sex	(0010, 0040)	2	CS 1	Patient.sex
Patient Comments	(0010, 4000)	3	LT 1	Patient.comment

**Table 35 CT Image Storage SOP Class (SCU) – General Study Module**

Attribute Name	Tag	DICOM Type	Notes
Study Instance UID	(0020, 000D)	1	Treatment.UID (generated by Elekta Synergy™ for native treatments)
Study Date	(0008, 0020)	2	Empty
Study Time	(0008, 0030)	2	Empty
Referring Physicians Name	(0008, 0090)	2	Patient.doctor^^^^
Study ID	(0020, 0010)	2	Treatment.ID
Accession Number	(0008, 0050)	2	Empty
Study Description	(0008, 1030)	3	Treatment.Description

Table 36 CT Image Storage SOP Class (SCU) – General Series Module

Attribute Name	Tag	DICOM Type	Notes
Modality	(0008, 0060)	1	“CT”
Series Instance UID	(0020, 000E)	1	New UID generated for each export.
Series Number	(0020, 0011)	2	Internally generated unique field-specific number.(New at each export)
Protocol Name	(0018, 1030)	3	“XVI Synergy”
Series Description	(0008, 103E)	3	Field.Description
Patient Position	(0018, 5100)	2C	Empty if position not specified by operator

Table 37 CT Image Storage SOP Class (SCU) – General Equipment Module

Attribute Name	Tag	DICOM Type	Notes
Manufacturer	(0008, 0070)	2	“ELEKTA”
Station Name	(0008, 1010)	3	IF an Elekta Synergy™ acquired image: Acquiring Station Name, ELSE: “UNKNOWN” + any available origin detail.
Manufacturers Model Name	(0008, 1090)	3	“Elekta XVI”
Device Serial Number	(0018, 1000)	3	Elekta Synergy™ Station Serial Number (see Note IV)
Software Versions	(0018, 1020)	3	Software revision of EXPORTING Station

Table 38 CT Image Storage SOP Class (SCU) – General Image Module

Attribute Name	Tag	DICOM Type	Notes
Image Number	(0020, 0013)	2	An internally generated unique image number within the CT Image set exported. Starts at 0 and incremented by one for each slices ordered on
Patient Orientation	(0020, 0020)	2C	Empty
Image Date	(0008, 0023)	2C	Image acquisition date
Image Time	(0008, 0033)	2C	Image acquisition time
Image Type	(0008, 0008)	3	DERIVED\SECONDARY\AXIAL
Acquisition Date	(0008, 0022)	3	Image acquisition date
Acquisition Time	(0008, 0032)	3	Image acquisition time
Images in Acquisition	(0020, 1002)	3	1
Image Comments	(0020, 4000)	3	Image. comment

Table 39 CT Image Storage SOP Class (SCU) –Image Plane Module

Name	Tag	DICOM Type	Notes/Constraints
Pixel spacing	(0028,0030)	1	Option1: Pixel spacing of volume Option2: Same as reference scan (see <b>Note XVIII</b> )
Image Orientation (Patient)	(0020,0037)	1	Option1: Depends on Patient orientation set at treatment level.

			Option2: Same as reference scan (see <b>Note XVIII</b> )
Image Position (Patient)	(0020,0032)	1	Option1: Use internal origin Option2: Same as reference scan (see <b>Note XVIII</b> )
Slice Thickness	(0018,0050)	1	Option1: Distance between 2 consecutive slices. Option2: Same as reference scan (see <b>Note XVIII</b> )

Table 40 CT Image Storage SOP Class (SCU) –Image Pixel Module

Name	Tag	DICOM Type	Notes/Constraints
Samples per Pixel	(0028,0002)	1	See Table 41
Photometric Interpretation	(0028,0004)	1	
Rows	(0028,0010)	1	Option 1: Y dimension of volume Option 2: same as reference volume (see <b>Note XVIII</b> )
Columns	(0028,0011)	1	Option 1: Z dimension of volume Option 2: same as reference volume (see <b>Note XVIII</b> )
Bits Allocated	(0028,0100)	1	See Table 41
Bits Stored	(0028,0101)	1	
High Bit	(0028,0102)	1	
Pixel Representation	(0028,0103)	1	
Pixel Data	(7FE0,0010)	1	Used for viewer file creation( <b>Note IX</b> )
Planar Configuration	(0028,0006)	1C	See Table 41
Pixel Aspect Ratio	(0028,0034)	1C	

**Note XVI Internal coordinate system**

The reconstructed volume is manipulated internally using a room fixed coordinate system

Table 41 CT Image Storage SOP Class (SCU) –CT Image Module

Name	Tag	DICOM Type	Notes/Constraints
Image Type	(0008,0008)	1	DERIVED\SECONDARY\AXIAL
Samples per Pixel	(0028,0002)	1	1
Photometric Interpretation	(0028,0004)	1	MONOCHROME2
Bits Allocated	(0028,0100)	1	16
Bits Stored	(0028,0101)	1	16
High Bit	(0028,0102)	1	15
Rescale Intercept	(0028,1052)	1	Sri.ini[Dicom]RescaleIntercept
Rescale Slope	(0028,1053)	1	Sri.ini[Dicom]RescaleSlope
KVP	(0018,0060)	2	Image.Kv
Reconstruction Diameter	(0018,1100)	3	See <b>Note XVII</b>
Gantry/Detector Tilt	(0018,1120)	3	0
Exposure Time	(0018,1150)	3	Image.kVLength
X-ray Tube Current	(0018,1151)	3	Image.mA
Filter Type	(0018,1160)	3	Image.filtratn
Focal Spot	(0018,1190)	3	Image.foc_spot

**Note XVII Reconstruction Diameter:**

The values of reconstruction diameter are ruled by the field of view used during acquisition:

- Small : 25.6 cm
- Medium : 40.0 cm
- Large : 50.0 cm

**Table 42 CT Image Storage SOP Class (SCU) – SOP Common Module**

Attribute Name	Tag	DICOM Type	Notes/Constraints
SOP Class UID	(0008, 0016)	1	CT Image storage UID
SOP Instance UID	(0008, 0018)	1	Generate new at every export
Specific Character Set	(0008, 0005)	1C	Ignored
Instance Creation Date	(0008, 0012)	3	
Instance Creation Time	(0008, 0013)	3	
Instance Creator UID	(0008, 0014)	3	

**Note XVIII Export options:**

Option 1: The user can export the full volume reconstructed choosing a factor to the original slice thickness.

Option 2: The volume is re-sampled in the reference scan coordinate and dimensions. Overlaps where data is missing on the reconstructed volume (i.e. the reference scan is bigger or offset compare to the reconstructed volume) are filled with black pixels.

## D. Applied RT Image IOD and mapping to Elekta Synergy™ Database

### D.1 Import of RT Image

The modules selected from the RT Image IOD of DICOM for prescription import are given in Table 43. If a module is not listed, none of the attributes in that module is stored by Elekta Synergy™.

**Table 43 Applied Modules in the RTImage IOD for Import (SCP Role)**

IE	MODULE	USAGE
Patient	Patient	M
Study	General Study	M
Series	RT Series	M
Equipment	General equipment (Ignored)	M
Image	General image	M
	Image Pixel	M
	RT Image	M
	SOP Common	M

### D.2 RT Image IOD Modules

Table 44 to Table 50 specify, for each of the applied modules above, the attributes stored by Elekta Synergy™, further details of mapping onto the Elekta Synergy™ database, and any attribute specific constraints applicable to their use.

Ignored attributes are not stored into the Elekta Synergy™ patient database. **However, all DICOM objects must conform to the DICOM standard.** If any part of a RT Image does not conform to the standard then that prescription is not saved into the database and the storage request is rejected. Thus, Elekta Synergy™ performs validation of the entire applied IOD. I.e. where attributes irrelevant to Elekta Synergy™ are included in a message, they must still have values that are valid according to the DICOM standard. Storage requests containing invalid attributes will be REJECTED. (See Table 71, **Status Code A901**).

Table 44 RT Image Storage SOP Class (SCP) – Patient Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Patients Name	(0010,0010)	PN 1	2	Split into Patient.first_name, Patient.last_name, Patient.mid_name (Prefix, Suffix not stored). See Note XIX.
Patient ID	(0010, 0020)	LO 1	2	Patient.id See Note XX
Patient's Birth Date	(0010, 0030)	DA 1	2	Patient.birth_date
Patients Sex	(0010, 0040)	CS 1	2	Patient.sex
Referenced Patient Sequence	(0008, 1120)	SQ 1	3	Ignored
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	
Patient's Birth Time	(0010, 0032)	TM 1	3	
Other Patient IDs	(0010, 1000)	LO 1-N	3	
Other Patient Names	(0010, 1001)	PN 1-N	3	
Ethnic Group	(0010, 2160)	SH 1	3	
Patient Comments	(0010, 4000)	LT 1	3	

**Note XIX Handling of Empty Patient Identification Attributes in a RT Image object**

The Patient ID (0010, 0020) and Patient Name (0010, 0010) attributes of the Patient Module are specified by DICOM as Type 2 and so may legally have zero length.

As a safety measure, however, **Elekta Synergy™** treats these attributes as Type 1 and will REJECT any RT Image Storage request containing zero length values for these attributes. Which means these RT Images won't enter the Elekta Synergy™ DICOM Transit database. (See **Table 71, Status Code C001**).

**Note XX Patient ID Already Exists in Elekta Synergy™ Database**

If a patient with the Patient ID specified in the RT Image Storage request already exists in the Elekta Synergy™ Main database, no further Patient Module attributes in the request will be imported. The check for an existing Patient ID is insensitive to case or leading/trailing spaces.

Table 45 RT Image Storage SOP Class (SCP) – General Study Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Study Instance UID	(0020, 000D)	UI 1	1	Treatment.dicom_uid
Study Date	(0008, 0020)	DA 1	2	Ignored
Study Time	(0008, 0030)	TM 1	2	
Referring Physicians Name	(0008, 0090)	PN 1	2	
Study ID	(0020, 0010)	SH 1	2	Treatment.id
Accession Number	(0008, 0050)	SH 1	2	See Note XXI
Study Description	(0008, 1030)	LO 1	3	Treatment.descrip
Physician(s) of Record	(0008, 1048)	PN 1-N	3	Ignored
Name of Physician(s) Reading Study	(0008, 1060)	PN 1-N	3	
Referenced Study Sequence	(0008, 1110)	SQ 1	3	
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	

**Note XXI Handling of Empty Study ID Attribute**

If a the RT Plan has been previously imported

An incrementing counter is prepended to the treatment id then ":" and one of the following

The applied Study ID (0020, 0010) is specified by DICOM as Type 2 and so may legally have zero length. This field is normally used by Elekta Synergy™ to identify the Treatment to be created or updated.

In the situation where the Study ID attribute is empty, Elekta Synergy™ will attempt to use the Accession Number (0008, 0050, Type 2) attribute as a Treatment ID instead. In such cases it will also append the Treatment Description with the text ":TRTID derived (Accession No.)" to assist the operator.

In the situation where both the Study ID and Accession Number attributes are empty, Elekta Synergy™ will use the last 16 digits of the Study Instance UID (0020, 000D) as a Treatment ID. In such cases it will also append the Treatment Description with the text ":TRTID derived (StudyInstanceUID.)" to assist the operator.

Extreme caution is advised when handling data with limited Study identification information present. It is the responsibility of the Elekta Synergy™ operator to ensure that incoming image data containing an empty Study ID attribute is correctly identified and qualified before relocation into the main Elekta Synergy™ Clinical database.

Table 46 RT Image SOP Class (SCP) – RT Series Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Modality	(0008, 0060)	CS 1	1	Ignored
Series Instance UID	(0020, 000E)	UI 1	1	Field.dicom_uid
Series Number	(0020, 0011)	IS 1	2	Ignored
Series Description	(0008, 103E)	LO 1	3	Field.description
Referenced Study Component Sequence	(0008, 1111)	SQ 1	3	Ignored
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	



**NoteXXII: Field.ID during RT Image import**

If the plan referenced by this RT image (Referenced RT Plan Sequence(300C,0002)) has been previously imported, the RT Image will be copied to the field created for the beam referenced by the beam number (Referenced Beam number (300C, 0006)) see Note XXVI.

If the plan describing the Beam referenced by the beam number (Referenced Beam number (300C, 0006)) has not been imported a field will be created with as an ID the beam number and the series description appended.

If the beam number (Referenced Beam number (300C, 0006)) is not present we use as Field.ID the prefix “:RTIMAGE” prefixed by an incrementing counter.

Extreme caution is advised when handling data with limited Series identification information present. It is the responsibility of the Elekta Synergy™ operator to ensure that incoming image data containing an empty Series Number attribute is correctly identified and qualified before relocation into the main Elekta Synergy™ Clinical database.

**Table 47 RT Image Storage SOP Class (SCP) –General Image Module**

Name	Tag	Type	VR, VM	Notes/Constraints
Instance Number	(0020,0013)	2	IS 1	Ignored
Patient Orientation	(0020,0020)	2C	CS 2	Image.orient
Content Date	(0008,0023)	2C	DA 1	Ignored
Content Time	(0008,0033)	2C	TM 1	
Image Type	(0008,0008)	3	CS 1-n	
Acquisition Number	(0020,0012)	3	IS 1	
Acquisition Date	(0008,0022)	3	DA 1	Image.Date. (if not present use date of import)
Acquisition Time	(0008,0032)	3	TM 1	Image.time (if not present use time of import)
Acquisition Datetime	(0008,002A)	3	DT 1	Ignored
Referenced Image Sequence	(0008,1140)	3	SQ 1	
>Referenced SOP Class UID	(0008,1150)	1C	UI 1	
>Referenced SOP Instance UID	(0008,1155)	1C	UI 1	
>Referenced Frame Number	(0008,1160)	3	IS 1-n	
>Purpose of Reference Code Sequence	(0040,A170)	3	SQ 1	
Derivation Description	(0008,2111)	3	ST 1	
Derivation Code Sequence	(0008,9215)	3	SQ 1	
Source Image Sequence	(0008,2112)	3	SQ 1	
>Referenced SOP Class UID	(0008,1150)	1C	UI 1	
>Referenced SOP Instance UID	(0008,1155)	1C	UI 1	
>Referenced Frame Number	(0008,1160)	3	IS 1-n	
>Purpose of Reference Code Sequence	(0040,A170)	3	SQ 1	
Referenced Waveform Sequence	(0008,113A)	3	SQ 1	
Images in Acquisition	(0020,1002)	3	IS 1	

Image Comments	(0020,4000)	3	LT 1	Image.comment
Quality Control Image	(0028,0300)	3	CS 1	Ignored
Burned In Annotation	(0028,0301)	3	CS 1	
Lossy Image Compression	(0028,2110)	3	CS 1	
Icon Image Sequence	(0088,0200)	3	SQ 1	
Presentation LUT Shape	(2050,0020)	3	CS 1	

Table 48 RT Image Storage SOP Class (SCP) –Image Pixel Module

Attribute Name	Tag	DICOM Type	Notes
Samples per Pixel	(0028, 0002)	1	<b>Assumed to be 1.</b>
Photometric Interpretation	(0028, 0004)	1	<b>MONOCHROME2.</b>
Rows	(0028, 0010)	1	Image.Height
Columns	(0028, 0011)	1	Image.Width
Bits Allocated	(0028, 0100)	1	Bits Allocated is 8 or 16
Bits Stored	(0028, 0101)	1	8 to 16
High Bit	(0028, 0102)	1	7 to 15
Pixel Representation	(0028, 0103)	1	Used to determine pixel scaling behaviour
Pixel Data	(7FE0, 0010)	1	Image pixel data interpreted.
Planar Configuration	(0028, 0006)	1C	<b>Assumed to be 0.</b>
Pixel Aspect Ratio	(0028, 0034)	1C	Image.Aspect

Table 49 RT Image Storage SOP Class (SCP) –RT Image Module

Name	Tag	Type	Notes/Constraints
Samples per Pixel	(0028,0002)	1	US 1
Photometric Interpretation	(0028,0004)	1	CS 1
Bits Allocated	(0028,0100)	1	US 1
Bits Stored	(0028,0101)	1	US 1
High Bit	(0028,0102)	1	US 1
Pixel Representation	(0028,0103)	1	US 1
RT Image Label	(3002,0002)	1	SH 1
RT Image Name	(3002,0003)	3	LO 1
RT Image Description	(3002,0003)	3	ST 1
Operators' Name	(0008,1070)	2	PN 1-n
Image Type	(0008,0008)	1	CS 1-n
Conversion Type	(0008,0064)	2	CS 1
Reported Values Origin	(3002,000A)	2C	CS 1
RT Image Plane	(3002,000C)	1	CS 1
X-Ray Image Receptor Translation	(3002,000D)	3	DS 3
X-Ray Image Receptor Angle	(3002,000E)	2	DS 1
RT Image Orientation	(3002,0010)	2C	DS 6
Image Plane Pixel Spacing	(3002,0011)	2	DS 2
RT Image Position	(3002,0012)	2	DS 2

Radiation Machine Name	(3002,0020)	2	SH 1	
Primary Dosimeter Unit	(300A,00B3)	2	CS 1	
Radiation Machine SAD	(3002,0022)	2	DS 1	
Radiation Machine SSD	(3002,0024)	3	DS 1	
RT Image SID	(3002,0026)	2	DS 1	
Source to Reference Object Distance	(3002,0028)	3	DS 1	
Referenced RT Plan Sequence	(300C,0002)	3	SQ 1	
>Referenced SOP Class UID	(0008,1150)	1C	UI 1	
>Referenced SOP Instance UID	(0008,1155)	1C	UI 1	
Referenced Beam Number	(300C,0006)	3	IS 1	Field.ID See NoteXXII: Field.beam_number
Referenced Fraction Group Number	(300C,0022)	3	IS 1	Fraction.ID
Fraction Number	(3002,0029)	3	IS 1	Ignored
Start Cumulative Meterset Weight	(300C,0008)	3	DS 1	
End Cumulative Meterset Weight	(300C,0009)	3	DS 1	
Exposure Sequence	(3002,0030)	3	SQ 1	
>Referenced Frame Number	(0008,1160)	1C	IS 1-n	
>KVP	(0018,0060)	1C	DS 1	Image.Kv
>X-Ray Tube Current	(0018,1151)	2C	IS 1	Image.mA
>Exposure Time	(0018,1150)	2C	IS 1	Image.kVlength
>Meterset Exposure	(3002,0032)	2C	DS 1	Ignored
>Diaphragm Position	(3002,0034)	3	DS 4	
>Beam Limiting Device Sequence	(300A,00B6)	3	SQ 1	
>>RT Beam Limiting Device Type	(300A,00B8)	1C	CS 1	
>>Source to Beam Limiting Device Distance	(300A,00BA)	3	DS 1	
>>Number of Leaf/Jaw Pairs	(300A,00BC)	1C	IS 1	
>>Leaf Position Boundaries	(300A,00BE)	2C	DS 3-n	
>>Leaf/Jaw Positions	(300A,011C)	1C	DS 2-2n	
>Applicator Sequence	(300A,0107)	3	SQ 1	
>>Applicator ID	(300A,0108)	1C	SH 1	
>>Applicator Type	(300A,0109)	1C	CS 1	
>>Applicator Description	(300A,010A)	3	LO 1	
>Number of Blocks	(300A,00F0)	1C	IS 1	
>Block Sequence	(300A,00F4)	2C	SQ 1	
>>Block Tray ID	(300A,00F5)	3	SH 1	
>>Source to Block Tray Distance	(300A,00F6)	2C	DS 1	
>>Block Type	(300A,00F8)	1C	CS 1	
>>Block Divergence	(300A,00FA)	2C	CS 1	
>>Block Mounting Position	(300A,00FB)	3	CS 1	
>>Block Number	(300A,00FC)	1C	IS 1	
>>Block Name	(300A,00FE)	3	LO 1	
>>Material ID	(300A,00E1)	2C	SH 1	
>>Block Thickness	(300A,0100)	3	CS 1	
>>Block Number of Points	(300A,0104)	2C	IS 1	
>>Block Data	(300A,0106)	2C	DS 2-2n	
Gantry Angle	(300A,011E)	3	DS 1	Frame.proj_angle
Beam Limiting Device Angle	(300A,0120)	3	DS 1	Ignored
Patient Support Angle	(300A,0122)	3	DS 1	
Table Top Eccentric Axis Distance	(300A,0124)	3	DS 1	

Table Top Eccentric Angle	(300A,0125)	3	DS1	
Table Top Vertical Position	(300A,0128)	3	DS 1	
Table Top Longitudinal Position	(300A,0129)	3	DS 1	
Table Top Lateral Position	(300A,012A)	3	DS 1	

**Table 50 RT Image Storage SOP Class (SCP) – SOP Common Module**

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
SOP Class UID	(0008, 0016)	UI 1	1	Ignored
SOP Instance UID	(0008, 0018)	UI 1	1	Image.dicom_uid
Specific Character Set	(0008, 0005)	CS 1-N	1C	Ignored
Instance Creation Date	(0008, 0012)	DA 1	3	
Instance Creation Time	(0008, 0013)	TM 1	3	
Instance Creator UID	(0008, 0014)	UI 1	3	

**Note XXIII Image.origin**

The field origin of the image table is populated with the sender AE title.

## E. Applied SC Image IOD and mapping to Elekta Synergy™ Database

### E.1 Import of SC Image

The modules selected from the Secondary Capture Image IOD table of DICOM for image import are given in Table 51. If a module is not listed, none of the attributes in that module is stored by Elekta Synergy™.

**Table 51 Applied Modules in the SC Image IOD for Import (SCP Role)**

IE	MODULE	USAGE
Patient	Patient	M
Study	General Study	M
Series	General Series	M
Image	General Image	M
	Image Pixel	M
	SC Image	M
	SOP Common	M

Table 52 to Table 58 specify, for each of the applied modules above, the attributes stored by Elekta Synergy™, and their mapping onto the Elekta Synergy™ database.

Ignored attributes are not stored into the Elekta Synergy™ patient database. **However, all DICOM objects must conform to the DICOM standard.** If any part of a Secondary Capture Image does not conform to the standard then that prescription is not saved into the database and the storage request is rejected. Thus, Elekta Synergy™ performs validation of the entire applied IOD. I.e. where attributes irrelevant to Elekta Synergy™ are included in a message, they must still have values that are valid according to the DICOM standard. Storage requests containing invalid attributes will be REJECTED. (See Table 71, **Status Code A901**).

Table 52 SC Image Storage SOP Class (SCP) – Patient Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Patients Name	(0010,0010)	PN 1	2	Split into Patient.first_name, Patient.last_name, Patient.mid_name (Prefix, Suffix not stored). (See Note XXIV , Note XXV).
Patient ID	(0010, 0020)	LO 1	2	Patient.id (See Note XXIV , Note XXV)
Patient's Birth Date	(0010, 0030)	DA 1	2	Patient.birth_date
Patients Sex	(0010, 0040)	CS 1	2	Patient.sex
Referenced Patient Sequence	(0008, 1120)	SQ 1	3	Ignored
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	
Patient's Birth Time	(0010, 0032)	TM 1	3	
Other Patient IDs	(0010, 1000)	LO 1-N	3	
Other Patient Names	(0010, 1001)	PN 1-N	3	
Ethnic Group	(0010, 2160)	SH 1	3	
Patient Comments	(0010, 4000)	LT 1	3	

**Note XXIV Handling of Empty Patient Identification Attributes**

The Patient ID (0010, 0020) and Patient Name (0010, 0010) attributes of the Patient Module are specified by DICOM as Type 2 and so may legally have zero length.

As a safety measure, however, **Elekta Synergy™** treats these attributes as Type 1 and will REJECT any Secondary Capture Image Storage request containing zero length values for these attributes. Which means these Secondary Capture Images won't enter the Elekta Synergy™ DICOM Transit database. (See **Table 71, Status Code C001**).

**Note XXV Patient ID Already Exists in Elekta Synergy™ Database**

If a patient with the Patient ID specified in the Secondary Capture Storage request already exists in the Elekta Synergy™ Main database, no further Patient Module attributes in the request will be imported. The check for an existing Patient ID is insensitive to case or leading/trailing spaces.

Table 53 SC Image Storage SOP Class (SCP) – General Study Module

Attribute Name	Tag	VR, VM	DICOM Type	Notes/Constraints
Study Instance UID	(0020, 000D)	UI 1	1	Treatment.dicom_uid
Study Date	(0008, 0020)	DA 1	2	Ignored
Study Time	(0008, 0030)	TM 1	2	
Referring Physicians Name	(0008, 0090)	PN 1	2	
Study ID	(0020, 0010)	SH 1	2	Treatment.id see Note XXVI
Accession Number	(0008, 0050)	SH 1	2	
Study Description	(0008, 1030)	LO 1	3	Treatment.descrip
Physician(s) of Record	(0008, 1048)	PN 1-N	3	Ignored
Name of Physician(s) Reading Study	(0008, 1060)	PN 1-N	3	
Referenced Study Sequence	(0008, 1110)	SQ 1	3	
>Referenced SOP Class UID	(0008, 1150)	UI 1	1C	
>Referenced SOP Instance UID	(0008, 1155)	UI 1	1C	

**Note XXVI Handling of Empty Study ID Attribute**

An incrementing counter is prepended to the treatment id then “:” and one of the following.

The applied Study ID (0020, 0010) is specified by DICOM as Type 2 and so may legally have zero length. This field is normally used by Elekta Synergy™ to identify the Treatment to be created or updated.

In the situation where the Study ID attribute is empty, Elekta Synergy™ will attempt to use the Accession Number (0008, 0050, Type 2) attribute as a Treatment ID instead. In such cases it will also append the Treatment Description with the text “:TRTID derived (Accession No.)” to assist the operator.

In the situation where both the Study ID and Accession Number attributes are empty, Elekta Synergy™ will use the last 16 digits of the Study Instance UID (0020, 000D) as a Treatment ID. In such cases it will also append the Treatment Description with the text “:TRTID derived (StudyInstanceUID.)” to assist the operator.

Extreme caution is advised when handling data with limited Study identification information present. It is the responsibility of the Elekta Synergy™ operator to ensure that incoming image data containing an empty Study ID attribute is correctly identified and qualified before relocation into the main Elekta Synergy™ Clinical database.

**Table 54 SC Image Storage SOP Class (SCP) – General Series Module**

Attribute Name	Tag	DICOM Type	Notes
Series Instance UID	(0020, 000E)	1	Field.UID . See Note XXVII below
Modality	(0008, 0060)	1	Ignored
Series Number	(0020, 0011)	2	Field.ID. See Note XXVII below
Laterality	(0020, 0060)	2C	Appended to Field.Site
Series Date	(0008, 0021)	3	Appended to Field.Description
Series Time	(0008, 0031)	3	Appended to Field.Description
Protocol Name	(0018, 1030)	3	Appended to Field.Description
Series Description	(0008, 103E)	3	Field.Description
Body Part Examined	(0018, 0015)	3	Field.Site
Patient Position	(0018, 5100)	2C	Field.orientation

**Note XXVII Handling of Empty Series Number Attribute**

The applied Series Number (0020, 0011) is specified by DICOM as Type 2 and so may legally have zero length. This field is normally used by Elekta Synergy™ to identify the Field to be created or updated.

In the situation where the Series Number attribute is empty, Elekta Synergy™ will use the last 16 digits of the Series Instance UID (0020, 000E) as a Field ID. In such cases it will also append the Field Description with the “:FLDID derived (SeriesInstanceUID)” to assist the operator.

**Note XXVIII Field ID**

For fields created from secondary images import the ID will start with the prefix “:SC IMAGE” and be prefixed by an incrementing counter. A new field will be created for every image imported.

Extreme caution is advised when handling data with limited Series identification information present. It is the responsibility of the Elekta Synergy™ operator to ensure that incoming image data containing an empty Series Number attribute is correctly identified and qualified before relocation into the main Elekta Synergy™ Clinical database.

Table 55 SC Image Storage SOP Class (SCP) –General Image Module

Name	Tag	Type	VR, VM	Notes/Constraints
Instance Number	(0020,0013)	2	IS 1	Ignored
Patient Orientation	(0020,0020)	2C	CS 2	Image.orient (using a single character based coding)
Content Date	(0008,0023)	2C	DA 1	Ignored
Content Time	(0008,0033)	2C	TM 1	
Image Type	(0008,0008)	3	CS 1-n	
Acquisition Number	(0020,0012)	3	IS 1	
Acquisition Date	(0008,0022)	3	DA 1	Image.Date. (if not present use date of import)
Acquisition Time	(0008,0032)	3	TM 1	Image.time (if not present use time of import)
Acquisition Datetime	(0008,002A)	3	DT 1	Ignored
Referenced Image Sequence	(0008,1140)	3	SQ 1	
>Referenced SOP Class UID	(0008,1150)	1C	UI 1	
>Referenced SOP Instance UID	(0008,1155)	1C	UI 1	
>Referenced Frame Number	(0008,1160)	3	IS 1-n	

Table 56 SC Image Storage SOP Class (SCP) – Image Pixel Module

Attribute Name	Tag	DICOM Type	Notes
Samples per Pixel	(0028, 0002)	1	Assumed to be 1.
Photometric Interpretation	(0028, 0004)	1	Assumed to be "MONOCHROME1" or "MONOCHROME2. See Note XXIX.
Rows	(0028, 0010)	1	Image.Height
Columns	(0028, 0011)	1	Image.Width
Bits Allocated	(0028, 0100)	1	Bits Allocated is 8 or 16
Bits Stored	(0028, 0101)	1	8 to 16
High Bit	(0028, 0102)	1	7 to 15
Pixel Representation	(0028, 0103)	1	Used to determine pixel scaling behaviour
Pixel Data	(7FE0, 0010)	1	Image pixel data interpreted.
Planar Configuration	(0028, 0006)	1C	Assumed to be 0
Pixel Aspect Ratio	(0028, 0034)	1C	Image.Aspect

**Note XXIX Stored Image Formats**

Elekta Synergy™ will **always** assume that pixel data is organised as 1 sample per pixel, either MONOCHROME1 or MONOCHROME2 interpretation and will store images accordingly.



**Table 57 SC Image Storage SOP Class (SCP) – SC Image Module**

Attribute Name	Tag	DICOM Type	Notes
Date of Secondary Capture	(0018, 1012)	3	Image.Acquisition Date
Time of Secondary Capture	(0018, 1014)	3	Image.Acquisition Time

**Table 58 SC Image Storage SOP Class (SCP) – SOP Common Module**

Attribute Name	Tag	DICOM Type	Notes
SOP Class UID	(0008, 0016)	1	Ignored.
SOP Instance UID	(0008, 0018)	1	Discarded. <b>A new UID is generated for Image.UID</b>
Specific Character Set	(0008, 0005)	1C	Ignored.

## E.2 Export of SC Image

The modules selected from the Secondary Capture Image IOD table of DICOM for image export are given in Table 59 below. If a module is not listed, none of the attributes in that module is sent by Elekta Synergy™.

**Table 59 Applied Modules in the SC Image IOD for Export (SCU Role)**

IE	Module	Usage
Patient	Patient	M
Study	General Study	M
Series	General Series	M
Equipment	General Equipment	U
	SC Equipment	M
Image	General Image	M
	Image Pixel	M
	SC Image	M
	SOP Common	M

Table 60 to Table 68 below specify the applied attributes for each module, and note their mappings from the Elekta Synergy™ database. If an attribute is not listed it is not sent by Elekta Synergy™. If an attribute is listed without Notes, there is a mapping from a directly equivalent Elekta Synergy™ database entry. Only the tags populated are listed.

Table 60 SC Image Storage SOP Class (SCU) – Patient Module

Attribute Name	Tag	DICOM Type	Notes
Patients Name	(0010,0010)	2	Patient.Last^ Patient.First^ Patient.Middle^^ (no Prefix or Suffix)
Patient ID	(0010, 0020)	2	Patient.ID
Patient's Birth Date	(0010, 0030)	2	Patient.birth_date
Patients Sex	(0010, 0040)	2	Patient.sex
Patient Comments	(0010, 4000)	3	Patient.comment

Table 61 SC Image Storage SOP Class (SCU) – General Study Module

Attribute Name	Tag	DICOM Type	Notes
Study Instance UID	(0020, 000D)	1	Treatment.UID (generated by Elekta Synergy™ for native treatments)
Study Date	(0008, 0020)	2	Empty
Study Time	(0008, 0030)	2	Empty
Referring Physicians Name	(0008, 0090)	2	Patient.doctor^^^^
Study ID	(0020, 0010)	2	Treatment.ID
Accession Number	(0008, 0050)	2	Empty
Study Description	(0008, 1030)	3	Treatment.Description

Table 62 SC Image Storage SOP Class (SCU) – General Series Module

Attribute Name	Tag	DICOM Type	Notes
Modality	(0008, 0060)	1	“CR”
Series Instance UID	(0020, 000E)	1	Field.UID (generated by Elekta Synergy™ for native fields)
Series Number	(0020, 0011)	2	IF Field ID is numeric: Field.ID, ELSE: an internally generated unique field-specific number.
Protocol Name	(0018, 1030)	3	“XVI Synergy”
Series Description	(0008, 103E)	3	Field.Description
Patient Position	(0018, 5100)	2C	Empty if position not specified by operator

Table 63 SC Image Storage SOP Class (SCU) – General Equipment Module

Attribute Name	Tag	DICOM Type	Notes
Manufacturer	(0008, 0070)	2	“ELEKTA”
Station Name	(0008, 1010)	3	IF an Elekta Synergy™ acquired image: Acquiring Station Name, ELSE: “UNKNOWN” + any available origin detail.
Manufacturers Model Name	(0008, 1090)	3	“Elekta XVI”
Device Serial Number	(0018, 1000)	3	Elekta Synergy™ Station Serial Number (see Note IV)
Software Versions	(0018, 1020)	3	Software revision of EXPORTING Station

**Note XXX Serial number:**

The station serial number is set through the initialisation file “sri.ini”

Table 64 SC Image Storage SOP Class (SCU) – SC Equipment Module

Attribute Name	Tag	DICOM Type	Notes
Conversion Type	(0008, 0064)	1	“DV”
Modality	(0008, 0060)	3	“CR”
Secondary Capture Device ID	(0018, 1010)	3	IF an Elekta Synergy™ acquired image: Acquiring Station Name, ELSE: “UNKNOWN” + any available origin detail.
Secondary Capture Device Manufacturer	(0018, 1016)	3	“ELEKTA”
Secondary Capture Device Manufacturer’s Model Name	(0018, 1018)	3	“Elekta XVI”
Secondary Capture Device Software Version	(0018, 1019)	3	Software revision of EXPORTING Station

Table 65 SC Image Storage SOP Class (SCU) – General Image Module

Attribute Name	Tag	DICOM Type	Notes
Image Number	(0020, 0013)	2	An internally generated database-unique image-specific number.
Patient Orientation	(0020, 0020)	2C	Empty if orientation not specified by operator
Image Date	(0008, 0023)	2C	Image acquisition date
Image Time	(0008, 0033)	2C	Image acquisition time
Image Type	(0008, 0008)	3	IF an Elekta Synergy™ acquired image: ORIGINAL\\PRIMARY ELSE: DERIVED\\SECONDARY
Acquisition Date	(0008, 0022)	3	Image acquisition date
Acquisition Time	(0008, 0032)	3	Image acquisition time
Images in Acquisition	(0020, 1002)	3	1
Image Comments	(0020, 4000)	3	Image. comment

Table 66 SC Image Storage SOP Class (SCU) –Image Pixel Module

Attribute Name	Tag	DICOM Type	Notes
Samples per Pixel	(0028, 0002)	1	1
Photometric Interpretation	(0028, 0004)	1	“MONOCHROME2”
Rows	(0028, 0010)	1	Image. height
Columns	(0028, 0011)	1	Image. width
Bits Allocated	(0028, 0100)	1	8 or 16
Bits Stored	(0028, 0101)	1	8 to 16
High Bit	(0028, 0102)	1	7 to 15
Pixel Representation	(0028, 0103)	1	0
Pixel Data	(7FE0, 0010)	1	
Planar Configuration	(0028, 0006)	1C	0
Pixel Aspect Ratio	(0028, 0034)	1C	Image.aspect
Smallest Image Pixel Value	(0028, 0106)	3	0
Largest Image Pixel Value	(0028, 0107)	3	255 or 65536

Table 67 SC Image Storage SOP Class (SCU) – SC Image Module

Attribute Name	Tag	DICOM Type	Notes
Date of Secondary Capture	(0018, 1012)	3	Image acquisition date
Time of Secondary Capture	(0018, 1014)	3	Image acquisition time

Table 68 SC Image Storage SOP Class (SCU) – SOP Common Module

Attribute Name	Tag	DICOM Type	Notes
SOP Class UID	(0008, 0016)	1	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008, 0018)	1	Image.UID (generated by Elekta Synergy™ for natively acquired images, and images imported from any source, including DICOM)
Instance Creation Date	(0008, 0012)	3	Date of export
Instance Creation Time	(0008, 0013)	3	Time of export
Instance Creator UID	(0008, 0014)	3	Derived from 6 digit Elekta Synergy™ workstation serial number. 1.3.46.423632 .<abcxyz>

## F. Extended Image Import Capability

In addition to the SOP classes supported by Elekta Synergy™ as SCP listed in Table 1 on page 9, above, the Elekta Synergy™ AE has the optional ability to store images of types other than Secondary Capture.

This feature is provided to extend the potential usefulness of the system as a general-purpose image viewing station, and is configurable to be enabled or disabled.

**NOTE:** The viewing, analysis, processing and printing functions within Elekta Synergy™ are primarily designed for portal images acquired by the Elekta Synergy™ system. When applied to images that are sent to Elekta Synergy™ by means of DICOM, in particular from modalities other than Portal Imagers, some of these functions may not perform optimally or may not be relevant.

When the capability is enabled the following additional SOP classes are supported by Elekta Synergy™ as SCP:

**Table 69 Additional SOP Classes supported by Elekta Synergy™ as SCP (Extended Import Option Enabled)**

SOP Class Name	UID
CR Image Storage - STORE	1.2.840.10008.5.1.4.1.1.1
MR Image Storage - STORE	1.2.840.10008.5.1.4.1.1.4

The modules selected from the Image IOD's for Extended Image Import are given in Table 70 below. If a module is not listed, none of the attributes in that module is stored by Elekta Synergy™.

**Table 70 Applied Modules in the Image IOD for Import (SCP Role: Extended Import)**

IE	Module	Usage
Patient	Patient	M
Study	General Study	M
Series	General Series	M
Image	General Image	M
	Image Pixel	M
	SOP Common	M

For the modules listed in Table 70, the attributes stored by Elekta Synergy™, and their mapping onto the Elekta Synergy™ database are as listed in the respective tables in Section A.2 above.

### F.1 C-STORE Conformance when Extended Import is enabled.

With Extended Import enabled, Elekta Synergy™ will provide standard conformance as a Conformance Level 0 Storage SCP for Secondary Capture.

For the additional SOP classes listed in Table 69 above, however, note the following:

- Should the images be re-exported, they will be exported as Secondary Capture, not as the original SOP class (the new SOP Instance UID generated at Storage time will be used).

## G. C-STORE Response Status Codes

Table 71 below lists the specific status code values returned by Elekta Synergy™ in a C-STORE response.

**Table 71 C-STORE Status Codes**

Service Status	Further Meaning	Status Code Values	Notes
Refused	Out of Resources	A7xx	
	- Dicom object already present in Elekta Synergy™ DICOM Transit database	A705	
	- No File set available (can't create or access)	A706	
	- The file set was locked for a period longer than timeout	A707	
Error	Data Set does not match SOP Class	A9xx	
	- Invalid Dicom message	A901	
Error	Cannot Understand	Cxxx	See Note I
	- Missing Patient Identification data	C001	
	- Non 16 Bit Image	C01B	
	- Image too small (number of rows and columns)	C01C	
	- Plan contain multiple isocenter	C01D	
Success		0000	